FLUKE

MP MASTER
MA25732

GOOGLE

6080A/82A

SYNTHESIZED RF SIGNAL GENERATOR

Operator Manual

P/N 861034
MAY 1990
©1990 John Fluke Mfg. Co., Inc. all rights reserved. Litho in U.S.A.

FLUKE

WARRANTY

Notwithstanding any provision of any agreement the following warranty is exclusive:

The JOHN FLUKE MFG. CO., INC., warrants each instrument it manufactures to be free from defects in material and workmanship under normal use and service for the period of 1-year from date of purchase. This warranty extends only to the original purchaser. This warranty shall not apply to fuses, disposable batteries (rechargeable type batteries are warranted for 90-days), or any product or parts which have been subject to misuse, neglect, accident, or abnormal conditions of operations.

In the event of failure of a product covered by this warranty, John Fluke Mfg. Co., Inc., will repair and calibrate an instrument returned to an authorized Service Facility within 1 year of the original purchase; provided the warrantor's examination discloses to its satisfaction that the product was defective. The warrantor may, at its option, replace the product in lieu of repair. With regard to any instrument returned within 1 year of the original purchase, said repairs or replacement will be made without charge. If the failure has been caused by misuse, neglect, accident, or abnormal conditions of operations, repairs will be billed at a nominal cost. In such case, an estimate will be submitted before work is started, if requested.

THE FOREGOING WARRANTY IS IN LIEU OF ALL OTHER WARRANTIES, EXPRESS OR IMPLIED, INCLUDING BUT NOT LIMITED TO ANY IMPLIED WARRANTY OF MERCHANTABILITY, FITNESS, OR ADEQUACY FOR ANY PARTICULAR PURPOSE OR USE. JOHN FLUKE MFG. CO., INC., SHALL NOT BE LIABLE FOR ANY SPECIAL, INCIDENTAL, OR CONSEQUENTIAL DAMAGES, WHETHER IN CONTRACT, TORT, OR OTHERWISE.

If any failure occurs, the following steps should be taken:

1. Notify the JOHN FLUKE MFG. CO., INC., or nearest Service facility, giving full details of the difficulty, and include the model number, type number, and serial number. On receipt of this information, service data, or shipping instructions will be forwarded to you.

2. On receipt of the shipping instructions, forward the instrument, transportation prepaid. Repairs will be made at the Service Facility and the instrument returned, transportation prepaid.

SHIPPING TO MANUFACTURER FOR REPAIR OR ADJUSTMENT

All shipments of JOHN FLUKE MFG. CO., INC., instruments should be made via United Parcel Service or "Best Way"* prepaid. The instrument should be shipped in the original packing carton; or if it is not available, use any suitable container that is rigid and of adequate size. If a substitute container is used, the instrument should be wrapped in paper and surrounded with at least four inches of excelsior or similar shock-absorbing material.

CLAIM FOR DAMAGE IN SHIPMENT TO ORIGINAL PURCHASER

The instrument should be thoroughly inspected immediately upon original delivery to purchaser. All material in the container should be checked against the enclosed packing list. The manufacturer will not be responsible for shortages against the packing sheet unless notified immediately. If the instrument is damaged in any way, a claim should be filed with the carrier immediately. (To obtain a quotation to repair shipment damage, contact the nearest Fluke Technical Center.) Final claim and negotiations with the carrier must be completed by the customer.

The JOHN FLUKE MFG. CO., INC, will be happy to answer all applications or use questions, which will enhance your use of this instrument. Please address your requests or correspondence to: JOHN FLUKE MFG. CO., INC., P.O. BOX C9090, EVERETT, WASHINGTON 98206, ATTN: Sales Dept. For European Customers: Fluke (Holland) B.V., P.O. Box 2269, 5600 CG, Eindhoven, The Netherlands.

*For European customers, Air Freight prepaid.

John Fluke Mfg. Co., Inc., P.O. Box C9090, Everett, Washington 98206

Rev. 7/88

Table of Contents

SECTION	TITLE	PAGE
1	**INTRODUCTION AND SPECIFICATIONS**	**1-1**
1-1.	INTRODUCTION	1-1
1-2.	INSTRUCTION MANUALS	1-2
1-3.	6080A/82A Operator Manual	1-2
1-4.	6080A/82A Operator Reference Guide	1-2
1-5.	6080A/82A Remote Programming Reference Guide	1-2
1-6.	6080A/82A Special Functions Decal	1-2
1-7.	6080A and 6082A Service Manuals	1-3
1-8.	OPTIONS	1-3
1-9.	WARRANTY AND SERVICE INFORMATION	1-3
1-10.	SPECIFICATIONS	1-4
2	**INSTALLATION**	**2-1**
2-1.	INTRODUCTION	2-1
2-2.	UNPACKING AND INSPECTION	2-1
2-3.	RACK OR BENCH MOUNTING	2-1
2-4.	POWER REQUIREMENTS	2-1
2-5.	LINE VOLTAGE SELECTION AND FUSE REPLACEMENT	2-2
2-6.	CONNECTING TO LINE POWER	2-4
2-7.	INTERNAL/EXTERNAL FREQUENCY REFERENCE	2-4
2-8.	LOCAL AND REMOTE OPERATION	2-5
2-9.	POWER-ON SEQUENCE	2-5
3	**FEATURES**	**3-1**
3-1.	INTRODUCTION	3-1
3-2.	FRONT PANEL FEATURES	3-1
3-5.	REAR PANEL FEATURES	3-1
4	**FRONT PANEL OPERATION**	**4-1**
4-1.	INTRODUCTION	4-1
4-2.	RECALLING PREVIOUS INSTRUMENT SETTINGS AT POWER-UP	4-1
4-3.	ENTERING AND MODIFYING PARAMETERS	4-1

(continued on page ii)

SECTION		TITLE	PAGE
	4-4.	Entering Parameters Directly	4-2
	4-5.	Editing the Bright Digit	4-2
	4-6.	Incrementing and Decrementing by Step	4-3
4A	**RF OUTPUT FREQUENCY**		**4A-1**
	4A-1.	INTRODUCTION	4A-1
	4A-2.	SETTING RF OUTPUT FREQUENCY	4A-1
	4A-3.	SETTING RF OUTPUT FREQUENCY STEP SIZE	4A-2
	4A-4.	USING RF OUTPUT FREQUENCY RELATIVE MODE	4A-2
	4A-5.	ADJUSTING THE PHASE OF THE RF CARRIER	4A-3
	4A-6.	USING AN EXTERNAL FREQUENCY REFERENCE	4A-3
	4A-7.	RF OUTPUT FREQUENCY BANDS	4A-4
4B	**RF OUTPUT AMPLITUDE**		**4B-1**
	4B-1.	INTRODUCTION	4B-1
	4B-2.	SETTING RF OUTPUT AMPLITUDE	4B-1
	4B-3.	CONVERTING RF OUTPUT AMPLITUDE UNITS	4B-2
	4B-4.	SELECTING ALTERNATE dB REFERENCE UNITS	4B-2
	4B-5.	USING UNTERMINATED OUTPUT (EMF) MODE	4B-3
	4B-6.	SETTING RF OUTPUT AMPLITUDE STEP SIZE	4B-4
	4B-7.	USING RF AMPLITUDE RELATIVE MODE	4B-4
	4B-8.	ENABLING AND DISABLING RF OUTPUT	4B-6
	4B-9.	RF OUTPUT AMPLITUDE BANDS	4B-6
	4B-10.	USING RF OUTPUT AMPLITUDE FIXED-RANGE MODE	4B-7
	4B-11.	USING ALTERNATE OUTPUT COMPENSATION MODES	4B-8
	4B-12.	SELECTING ALTERNATE OUTPUT COMPENSATION DATA	4B-8
4C	**MODULATION**		**4C-1**
	4C-1.	INTRODUCTION	4C-1
	4C-2.	INTERNAL MODULATION OSCILLATOR	4C-1
	4C-3.	Setting Modulation Frequency and Step Size	4C-2
	4C-4.	Setting Modulation Level and Step Size	4C-3
	4C-5.	Enabling and Disabling Modulation Output	4C-4
	4C-6.	Selecting the Internal Modulation Waveform	4C-4
	4C-7.	Using the Extended Resolution Mode for Modulation Frequency	4C-5
	4C-8.	AMPLITUDE MODULATION (AM)	4C-5
	4C-9.	Setting AM Depth and AM Depth Step Size	4C-5
	4C-10.	Activating Internal AM	4C-6
	4C-11.	Activating External AM (AC Coupled)	4C-6
	4C-12.	Activating External AM (DC Coupled)	4C-7
	4C-13.	FREQUENCY AND PHASE MODULATION (FM/ϕM)	4C-7
	4C-14.	Setting FM/ϕM Deviation and FM/ϕM Step Size	4C-7
	4C-15.	Converting FM/ϕM Units	4C-9
	4C-16.	Activating Internal FM/ϕM	4C-10
	4C-17.	Activating External FM/ϕM (AC Coupled)	4C-10
	4C-18.	Activating External FM (DC Coupled)	4C-10
	4C-19.	FM Bands	4C-11
	4C-20.	Using Low Distortion and Fixed-Range FM Modes	4C-12
	4C-21.	Using Low Rate FM Mode	4C-13

(continued on page iii)

SECTION	TITLE	PAGE
4C-22.	Using High Rate ϕM Mode	4C-13
4C-23.	PULSE MODULATION	4C-14
4C-24.	Activating External Pulse Modulation	4C-14
4C-25.	Activating Internal Pulse Modulation	4C-14
4C-26.	Using the Mod Oscillator as a Pulse Generator	4C-14
4C-27.	Setting Pulse Width	4C-15
4D	**INSTRUMENT STATE MEMORY**	**4D-1**
4D-1.	ORGANIZATION OF INSTRUMENT STATE MEMORY	4D-1
4D-2.	STORING AND RECALLING INSTRUMENT STATES	4D-3
4D-3.	RECALLING A SEQUENCE OF INSTRUMENT STATES	4D-4
4D-4.	DIVIDING MEMORY INTO PARTITIONS	4D-4
4D-5.	WRITE-PROTECTING MEMORY LOCATIONS	4D-6
4D-6.	RESETTING ALL MEMORY LOCATIONS TO FACTORY DEFAULT	4D-6
4D-7.	STORING AND RECALLING SINGLE PARAMETERS	4D-6
4E	**SWEEP**	**4E-1**
4E-1.	INTRODUCTION	4E-1
4E-2.	SELECTING FREQUENCY OR AMPLITUDE SWEEP	4E-2
4E-3.	SUMMARY OF SWEEP MODES	4E-2
4E-4.	SELECTING SYMMETRIC OR ASYMMETRIC SWEEP	4E-3
4E-5.	SETTING SWEEP DWELL TIME	4E-3
4E-6.	FREQUENCY SWEEP	4E-4
4E-7.	Setting Frequency Sweep Width	4E-5
4E-8.	Setting Frequency Sweep Increment	4E-5
4E-9.	Digital Frequency Sweep Example	4E-6
4E-10.	AMPLITUDE SWEEP	4E-6
4E-11.	Setting Amplitude Sweep Width	4E-8
4E-12.	Setting Amplitude Sweep Increment	4E-8
4E-13.	Digital Amplitude Sweep Example	4E-9
4E-14.	CALIBRATING A RECORDER OR OSCILLOSCOPE	4E-10
4E-15.	ANALOG FREQUENCY SWEEP	4E-10
4F	**SPECIAL FUNCTIONS**	**4F-1**
4F-1.	INTRODUCTION	4F-1
4F-2.	ENABLING SPECIAL FUNCTIONS	4F-3
4F-3.	VIEWING ENABLED SPECIAL FUNCTIONS	4F-3
4F-4.	THE SPCL ANNUNCIATOR	4F-4
4F-5.	MISCELLANEOUS SPECIAL FUNCTIONS	4F-4
4F-6.	Disable Special Functions	4F-4
4F-7.	Restore Instrument Preset State	4F-4
4F-8.	Execute Self-Test and Display Self-Test Results	4F-4
4F-9.	Display Loaded Options	4F-4
4F-10.	Display Instrument ID and Software Revision Level	4F-4
4F-11.	Blank Front Panel Display	4F-5
4F-12.	Select Repeat Rate for Step Keys	4F-5
4F-13.	Configure Edit Knob and Step Keys	4F-5

(continued on page iv)

SECTION	TITLE	PAGE
4G	**ERROR AND STATUS REPORTING**	**4G-1**
4G-1.	GENERAL DESCRIPTION	4G-1
4G-2.	THE STATUS KEY	4G-1
4G-3.	DISPLAYING SELF-TEST STATUS AND CALIBRATION/COMPENSATION DATA	4G-2
5	**REMOTE OPERATION**	**5-1**
5-1.	INTRODUCTION	5-1
5-2.	SETTING UP THE IEEE-488 INTERFACE	5-1
5-3.	Address Setup Procedure	5-2
5-4.	Talker/Listener Mode Selection Procedure	5-2
5-5.	Compatibility Language Selection Procedure	5-3
5A	**REMOTE PROGRAMMING**	**5A-1**
5A-1.	INTRODUCTION	5A-1
5A-2.	COMMAND SYNTAX INFORMATION	5A-2
5A-3.	Parameter Syntax Rules	5A-2
5A-4.	Extra Space Characters	5A-3
5A-5.	Terminators	5A-3
5A-6.	Incoming Character Processing	5A-4
5A-7.	Response Message Syntax	5A-4
5A-8.	INPUT BUFFER OPERATION	5A-4
5A-9.	COMMANDS	5A-4
5A-10.	Multiple Commands	5A-5
5A-11.	Command Processing	5A-5
5A-12.	Command Restrictions	5A-5
5A-13.	Commands That Require the CAL|COMP Switch To Be Set	5A-5
5A-14.	REMOTE/LOCAL STATE TRANSITIONS	5A-6
5A-15.	CHECKING THE INSTRUMENT STATUS	5A-7
5A-16.	Serial Poll Status Byte (STB)	5A-7
5A-17.	BIT ASSIGNMENTS FOR THE STB AND SRE	5A-7
5A-18.	SERVICE REQUEST LINE (SRQ)	5A-9
5A-19.	SERVICE REQUEST ENABLE REGISTER (SRE)	5A-9
5A-20.	PROGRAMMING THE STB AND SRE	5A-10
5A-21.	Event Status Register (ESR)	5A-10
5A-22.	BIT ASSIGNMENTS FOR THE ESR AND ESE	5A-10
5A-23.	EVENT STATUS ENABLE REGISTER (ESE)	5A-12
5A-24.	PROGRAMMING THE ESR AND ESE	5A-12
5A-25.	Output Queue	5A-13
5A-26.	Error Queue	5A-13
5A-27.	Instrument Status Register (ISR)	5A-14
5A-28.	BIT ASSIGNMENTS FOR THE ISR, ISCR, AND ISCE	5A-14
5A-29.	INSTRUMENT STATUS CHANGE REGISTER (ISCR)	5A-14
5A-30.	INSTRUMENT STATUS CHANGE ENABLE REGISTER (ISCE)	5A-15
5A-31.	PROGRAMMING THE ISR, ISCR, AND ISCE	5A-15
5A-32.	Status Queue	5A-16
5A-33.	IEEE-488 INTERFACE CONFIGURATION	5A-16

(continued on page v)

SECTION	TITLE	PAGE
	5A-34. BUS COMMUNICATION OVERVIEW	5A-16
	5A-35. Definition: Queries and Commands	5A-17
	5A-36. Functional Elements of Commands	5A-17
	5A-37. Interface Messages	5A-19
	5A-38. THE IEEE-488 CONNECTOR	5A-21
	5A-39. REMOTE PROGRAM EXAMPLES	5A-22
	5A-40. Using the *OPC?, *OPC, and *WAI Commands	5A-22
	5A-41. Using the *DDT and *TRG Commands	5A-23
5B	**REMOTE COMMAND TABLES**	**5B-1**
	5B-1. REMOTE COMMAND SUMMARY	5B-1
	5B-2. REMOTE COMMANDS	5B-1
5C	**TALK-ONLY/LISTEN-ONLY OPERATION**	**5C-1**
	5C-1. INTRODUCTION	5C-1
	5C-2. TALK-ONLY OPERATION	5C-1
	5C-3. LISTEN-ONLY OPERATION	5C-2
	5C-4. LISTEN-ONLY/TALK-ONLY EXAMPLE	5C-2
5D	**COMPATIBILITY LANGUAGES**	**5D-1**
	5D-1. INTRODUCTION	5D-1
	5D-2. SELECTING THE ACTIVE LANGUAGE	5D-1
	5D-3. USING THE 6060 AND 6070 FAMILY LANGUAGES	5D-2
	5D-4. Incompatibilities	5D-2
	5D-5. Converting 6060 and 6070 Programs to Use the 6080 Language	5D-9
	5D-6. USING THE HP 8642 FAMILY LANGUAGE	5D-11
	5D-7. IEEE-488 (GPIB) Address	5D-11
	5D-8. IEEE-488 (GPIB) Interface Capabilities	5D-11
	5D-9. Data Input and Numeric Formatting	5D-12
	5D-10. Data Output	5D-12
	5D-11. HP8642 Commands that are Ignored	5D-12
	5D-12. RF Output Frequency	5D-12
	5D-13. Relative RF Frequency	5D-15
	5D-14. RF Frequency Sweep	5D-15
	5D-15. RF Output Amplitude	5D-16
	5D-16. EMF Units	5D-16
	5D-17. Relative Amplitude	5D-16
	5D-18. Amplitude Sweep	5D-16
	5D-19. AM/Pulse Modulation	5D-16
	5D-20. FM/ϕM	5D-16
	5D-21. Internal Modulation Oscillator	5D-17
	5D-22. Instrument Preset/Partial Preset	5D-18
	5D-23. Knob Control/Entry Off	5D-18
	5D-24. Step, Increment Set	5D-18
	5D-25. Save/Recall Register	5D-18
	5D-26. Special Functions	5D-19
	5D-27. Messages	5D-19

(continued on page vi)

SECTION	TITLE	PAGE
Appendix A		
	Instrument Preset State	A-1
Appendix B		
	Special Function Table	B-1
Appendix C		
	Rejected Entry Codes	C-1
Appendix D		
	Overrange/Uncal Status Codes	D-1
Appendix E		
	Self-Test Status Codes	E-1
Appendix F		
	Rear Panel AUX Connector Pinout	F-1
Appendix G		
	Fluke Sales and Service Centers	G-1

List of Tables

TABLE	TITLE	PAGE
1-1.	Specifications for Model 6080A	1-5
1-2.	Specifications for Model 6082A	1-12
2-1.	Standard Equipment	2-2
2-2.	Line Power Cord Types Available from Fluke	2-2
2-3.	Accessories	2-3
3-1.	Front Panel Features	3-3
3-2.	Rear Panel Features	3-12
4-1.	Step Size Defaults	4-3
4A-1.	Signal Generator Frequency Bands	4A-4
4B-1.	Relative Amplitude Unit Combinations	4B-5
4B-2.	RF Output Amplitude Bands	4B-6
4C-1.	FM/ϕM Deviation Limits (FM/ϕM Enabled)	4C-9
4C-2.	FM Band Limits	4C-11
4C-3.	FM Band Limits - Low Distortion Mode	4C-12
4D-1.	Non-Storable/Recallable Parameters	4D-2
4D-2.	Non-Volatile Memory Locations	4D-2
4F-1.	Special Function Codes	4F-2
4F-2.	Functions of Edit Knob and Step Keys	4F-5
4G-1.	Interpreting Status Codes	4G-2
5A-1.	Remote/Local State Transitions	5A-7
5A-2.	IEEE-488 Interface Function Subsets Supported	5A-9
5A-3.	Functional Elements of Commands	5A-18
5A-4.	Interface Messages that the Signal Generator Accepts	5A-19
5A-5.	Interface Messages that the Signal Generator Sends	5A-21
5B-1.	Remote Command Summary	5B-2
5B-2.	Units That Can Be Used With Remote Commands	5B-7
5B-3.	Remote Commands	5B-8
5D-1.	6060 Compatibility Language Codes and Special Functions	5D-3
5D-2.	6070 Compatibility Language Codes and Special Functions	5D-5
5D-3.	6060 and 6070 Compatibility Language Commands	5D-7
5D-4.	6060 and 6070 Compatibility Language Units	5D-10
5D-5.	IEEE-488 Interface Capibilities/HP8642 Language	5D-11
5D-6.	6080 to HP8642 Error Code Mapping	5D-13
5D-7.	HP8642 Commands that are Ignored	5D-14
5D-8.	HP8642 RF Output Frequency Commands not Accepted	5D-14
5D-9.	Frequency Sweep Commands Not Accepted	5D-15
5D-10.	Amplitude Sweep Commands Not Accepted	5D-17
5D-11.	FM/ϕM Commands Not Accepted	5D-17
5D-12.	HP8642 Special Functions Emulated	5D-19

List of Illustrations

FIGURES	TITLE	PAGE
2-1.	Line Power Cords Avaliable from Fluke	2-3
2-2.	Fuse/Line Voltage Selection Assembly	2-4
3-1.	Front Panel Features	3-2
3-2.	Rear Panel Features	3-11
5A-1.	Overview of Status Data Structure	5A-8
5A-2.	Bit Assignments for the STB and SRE	5A-9
5A-3.	Bit Assignments for ESR and ESE	5A-11
5A-4.	Bit Assignments for the ISR, ISCR, and ISCE	5A-14
5A-5.	IEEE-488 Connector and Pin Assignments	5A-21

Section 1
Introduction and Specifications

INTRODUCTION 1-1.

The 6080A and 6082A Synthesized RF Signal Generators are fully programmable, precision, synthesized signal sources. They are designed for applications that require good modulation, frequency and output level performance with excellent spectral purity. Both Signal Generators are well suited for testing a wide variety of rf components, sub-assemblies, and systems, including filters, amplifiers, mixers, and receivers, particularly off-channel radio testing.

Both models are called the Signal Generator in this manual. It is noted wherever information applies specifically to one model or the other.

Specifications of the Signal Generator are provided at the end of this section. Features of the Signal Generator include the following:

- Frequency range, in 1 Hz steps, as follows:

  6080A: 10 kHz to 1056 MHz
  6082A: 100 kHz to 2112 MHz

- Amplitude ranges as follows, with 0.1 dB resolution:

  6080A: +19 to -140 dBm for rf output frequencies below 512 MHz, and
  +17 to -140 dBm for rf output frequencies 512 MHz and above

  6082A: +16 to -140 dBm for rf output frequencies below 1056 MHz, and
  +13 to -140 dBm for rf output frequencies 1056 MHz and above

- Amplitude units accepted and displayed: dB, dBm, dBf, dBμV, dBmV, μV, mV, V, and EMF

- Internal and external modulation: AM, FM, ϕM, and pulse

- Internal 0.1 Hz to 200 kHz direct-digital synthesis modulation oscillator that provides sine, square, triangular, and pulse waveforms

- Digital frequency sweep and digital amplitude sweep

- Fifty storable and recallable instrument state memory locations

- Standard IEEE-488 (GPIB) Interface, complying with ANSI/IEEE Standards 488.1-1987 and 488.2-1987
- Software compatibility modes for emulation of Fluke 6060/6070 or Hewlett Packard HP8642A/B remote programming languages
- Closed-case calibration capabilities for frequency reference, AM, FM, and level

INSTRUCTION MANUALS 1-2.

The 6080A/82A Manual Set provides complete information for the operator and service or maintenance personnel. The set includes the following manuals:

- 6080A/82A Operator Manual, PN 861034
- 6080A/82A Operator Reference Guide, PN 882154
- 6080A/82A Remote Programming Reference Guide, PN 882147
- 6080A/82A Special Functions Decal, PN 860911
- 6080A Service Manual, PN 868914
- 6082A Service Manual, PN 881888

Each Signal Generator is shipped one each of the first four manuals above, plus the applicable Service Manual. The two reference guides and the special functions decal are packaged with this Operator Manual. You can order additional copies of the manuals, reference guides, or decal separately using the part number provided. For ordering instructions, refer to the Fluke Catalog, or contact a Fluke sales representative. A list of Fluke Sales and Service Centers is in Appendix G.

6080A/82A Operator Manual 1-3.

This 6080A/82A Operator Manual provides complete information for installing the Signal Generator and operating it from the front panel controls and in remote over the IEEE-488 Bus.

6080A/82A Operator Reference Guide 1-4.

The 6080A/82A Operator Reference Guide is a pocket-sized booklet that contains a summary of operating instructions from this Operator Manual, including a front and rear panel feature reference, special function codes, and status and error codes.

6080A/82A Remote Programming Reference Guide 1-5.

The 6080A/82A Remote Programming Reference Guide is a pocket-sized booklet that contains a summary of remote operating information, including syntax rules, remote commands, parameters, and responses, plus how to determine system status using the status byte and registers.

6080A/82A Special Functions Decal 1-6.

The 6080A/82A Special Functions Decal is an adhesive-backed reference card intended to be affixed to the top surface of the Signal Generator. The card contains a summary of the Special Functions that are activated by entering number codes with the numeric keypad.

6080A and 6082A Service Manuals 1-7.

These service manuals are maintenance guides for the Signal Generator. The following topics are included in the service manual:

- Theory of operation
- Closed-case calibration
- Performance testing
- Access procedures
- Troubleshooting and alignment
- Parts lists
- Schematic diagrams

OPTIONS 1-8.

Three options are available for the 6080A and the 6082A:

- 6080A-830 (or 6082A-830) Rear Output and Rear Modulation Input
- 6080A-130 (or 6082A-130) High-Stability Reference (see Specifications)
- 6080A-132 (or 6082A-132) Medium-Stability Reference (see Specifications)

All three options are factory-installable only. The -830 option moves the MOD OUTPUT, RF OUTPUT, and MODULATION INPUT connectors to the rear panel. The front panel connector holes are covered with plugs.

The way you operate the Signal Generator with the -130 or -132 option installed is the same as with the standard reference. Refer to the specifications for the change in time and temperature stability of each reference.

The service manual contains theory of operation and schematic diagrams for each option in the Options section.

WARRANTY AND SERVICE INFORMATION 1-9.

Each Signal Generator is warranted for a period of 1 year upon delivery to the original purchaser. The warranty is on the back of the title page of this manual.

Factory authorized service for the Signal Generator is available at selected Fluke Technical Service Centers. For service, return the Signal Generator to the nearest Fluke Technical Service Center. The local service center will handle transportation to and from the selected service center as required. A complete list of Fluke Sales and Technical Service Centers is provided in Appendix G.

To reship the Signal Generator, use its original shipping carton. If the original carton is not available, use a container that provides adequate protection during shipment. Protect the Signal Generator with at least three inches of shock-absorbing material on all sides of the container. Do not use loose fill to pad the shipping container. Loose fill allows the Signal Generator to settle to one corner of the shipping container, which could result in damage during shipment.

After-warranty service is available, but you may choose to repair the Signal Generator using the information in the Troubleshooting section of the service manual and the Module Exchange Program. Refer to the Fluke catalog or contact a Technical Service Center representative for the module exchange procedure.

SPECIFICATIONS 1-10.

Table 1-1 lists specifications for Model 6080A. Table 1-2 lists specifications for Model 6082A. Specifications are valid after a warm-up period of 20 minutes. Specifications remain valid after two years only if the Signal Generator is calibrated at that time as described in the service manual, and every two years or more frequently thereafter. In the Specification tables, dBc refers to decibels relative to the amplitude of the carrier.

Table 1-1. Specifications for Model 6080A

FREQUENCY

Range: 10 kHz to 1056 MHz. (Also see Internal Modulation Oscillator for coverage from 0.1 Hz to 200 kHz.)
Frequency Bands: The carrier frequency band endpoints are shown below.

BAND DESIGNATION	APPROXIMATE CARRIER FREQUENCY BAND (MHz)	SPECIFIC CARRIER FREQUENCY BAND (MHz)
A	0.01 to 15	0.01 to 14.999,999
B	15 to 32	15 to 31.999,999
C	32 to 64	32 to 63.999,999
D	64 to 128	64 to 127.999,999
E	128 to 256	128 to 255.999,999
F	256 to 512	256 to 511.999,999
G	512 to 1056	512 to 1056

Resolution: 1 Hz
Display Resolution: 10 digits
Stability: Same as Internal Reference Oscillator

10 MHz INTERNAL REFERENCE OSCILLATOR

Type: Temperature Compensated Crystal Oscillator (TCXO)
Temperature Stability: Less than ±1 ppm p-p over the range 0 to +50°C
Typical Aging Rate: Less than ±1 ppm/yr
Reference Output: 10 MHz, >0 dBm for 50Ω load, available at the rear-panel REF OUT connector.

PROVISION FOR EXTERNAL REFERENCE

The rear panel REF IN connector accepts an external source of 10 MHz ±10 ppm sine wave, 0.2 to 2.0V rms for a 50Ω load. One alternate external reference frequency setting of 1, 2, or 5 MHz is available at a time, through Special Function 761 or a remote command. The default alternate reference frequency is 5 MHz. See the Service Manual for setting internal DIP switches for use with a 1 or 2 MHz external reference.

AMPLITUDE

Range: +19 to -140 dBm for rf output frequency <512 MHz.
+17 to -140 dBm for rf output frequency >512 MHz.
Resolution: 0.1 dB (0.1% or 1 nV in volts). Annunciators for dB, dBm, V, mV, µV, dBf, dBµV, dBmV, and EMF
Display Resolution: 3 1/2 digits

Accuracy (0 to 50°C):

FREQUENCY (MHz)	AMPLITUDE IN dBm +19 +17 -127 -140
0.01 to 0.1	±3 dBm
0.1 to 0.4	±2 dBm ±3 dBm
0.4 to 512	±1 dBm ±3 dBm
512 to 1056	±1 dBm ±3 dBm

Table 1-1. Specifications for Model 6080A (cont.)

Source SWR: <1.5:1 below +6 dBm
<2.0:1 above +6 dBm
Flatness (0 to 50°C): ±0.75 dB at +10 dBm, for frequencies >0.1 MHz
Intermodulation Distortion (Amplitude of +4 dBm, CW only):

FREQUENCY (MHz)	SPACING 1 kHz	25 kHz
0.01 to 128 MHz	-60 dBc	-80 dBc
128 to 512 MHz	-65 dBc	-75 dBc
512 to 1056 MHz	-65 dBc	-70 dBc

SPECTRAL PURITY (CW ONLY)
Spurious Signals: <-100 dBc for offsets greater than 10 kHz.
Fixed-frequency spurious signals are <-100 dBc or <-140 dBm, whichever is greater.
Harmonics: <-30 dBc for amplitudes less than +13 dBm.
Sub-harmonics: None.
Power Line Spurious Signals (offsets less than 10 kHz): <-56 dBc
Residual FM: (NOTE 1)

FREQUENCY BAND (MHz)	RESIDUAL FM 0.3 to 3 kHz	0.05 to 15 kHz
0.01 to 15	0.3	0.6
15 to 32	0.3	0.6
32 to 64	0.3	0.6
64 to 128	0.3	0.6
128 to 256	0.3	0.6
256 to 512	0.7	1.2
512 to 1056	1.5	2.5

SSB Phase Noise: (NOTE 1)

CARRIER FREQUENCY BAND (MHz)	OFFSET FREQUENCY 1 kHz (dBc/Hz)	20 kHz (dBc/Hz)	100 kHz (dBc/Hz)
0.01 to 15	-112	-138	-138
15 to 32	-124	-145	-146
32 to 64	-118	-144	-146
64 to 128	-112	-144	-145
128 to 256	-106	-141	-144
256 to 512	-100	-136	-142
512 to 1056	-94	-130	-138

Residual AM (0.05 to 15 kHz Band): <-80 dBc (.01%)

NOTE 1: *Allowable operating modes CW, AM, FM (Peak dev. <1.5% of max in operating band), øM (same comment as FM), Pulse.*

Table 1-1. Specifications for Model 6080A (cont.)

AMPLITUDE MODULATION

Depth Range: 0% to 99.9% for rf output level <+10 dBm.
AM Resolution: 0.1%
AM Display: 3 digits
AM Accuracy: ±(2% + 4% of setting) for rate = 1 kHz and depth <90%
AM Distortion (Rate = 1 kHz) (NOTE 2): <1.5% THD to 30% AM
<3% THD to 70% AM
<5% THD to 90% AM

AM 3-dB Bandwidth (NOTE 2): AC-coupled AM, 20 Hz to 50 kHz
DC-coupled AM, dc to 50 kHz

Incidental ØM: <0.20 radian for rates
<1 kHz and <30% AM

FREQUENCY MODULATION (NOTE 3)

FM Display Ranges: 0 to 999 Hz
1 to 9.99 kHz
10 to 99.9 kHz
100 to 999 kHz
1 to 4.00 MHz
FM Display Resolution: 3 digits

Maximum Deviation:

FREQUENCY BAND (MHz)	MAXIMUM DEVIATION	
	DC-COUPLED FM	AC-COUPLED FM (THE SMALLER OF)
0.01 to 15	500 kHz	500 kHz or fmod x 5,000
15 to 32	125 kHz	125 kHz or fmod x 1,250
32 to 64	250 kHz	250 kHz or fmod x 2,500
64 to 128	500 kHz	500 kHz or fmod x 5,000
128 to 256	1 MHz	1 MHz or fmod x 10,000
256 to 512	2 MHz	2 MHz or fmod x 20,000
512 to 1056	4 MHz	4 MHz or fmod x 40,000

FM Distortion:
Standard Mode: <2% for 0.5 to 1.0 times maximum deviation; <1% for <0.5 times maximum deviation. Applies for rates of 50 Hz to 50 kHz.
Low-Distortion Mode (Special Function 731): <0.33% for <= 3.5 kHz peak deviation and rates 0.3 to 3 kHz.
FM Resolution: 3 digits.
FM Accuracy: ±(5% of setting + 10 Hz) for rates of 0.05 to 50 kHz

NOTE 2: AM specifications apply where RF output frequency - modulation frequency is greater than 150 kHz.

NOTE 3: FM specifications apply where: rf output frequency - deviation) >150 kHz, and rf output frequency - modulation rate >150 kHz.

Table 1-1. Specifications for Model 6080A (cont.)

FM 3-dB Bandwidth:

DEVIATION	COUPLING	
	INTERNAL AC	EXTERNAL AC (DC)
0% to 25% Maximum	20 Hz to 175 kHz	20 Hz (dc) to 175 kHz
25% to 100% Maximum	20 Hz to 100 kHz	20 Hz (dc) to 100 kHz

Incidental AM: <1% depth for peak deviation <100 kHz at 1 kHz rate and carrier frequency >0.5 MHz
DC-Coupled FM Center Frequency Error, at 1 GHz, after dcFM internal cal, and without any FM range changes: <(.1% of dev + 500 Hz)
Low-Rate External AC-Coupled FM (Special Function 711):

FREQUENCY BAND (MHz)	MAX DEV, IN kHz (AT 10 Hz RATE)	
	SINE WAVE	SQUARE WAVE
0.01 to 15	80	40
15 to 32	20	10
32 to 64	40	20
64 to 128	80	40
128 to 256	160	80
256 to 512	320	160
512 to 1056	640	320

Droop: <30% on a 5 Hz square wave
3-dB Bandwidth: 0.5 Hz to 100 kHz (typical)
Maximum dc Input: ±10 mV
Incidental AM: <1% AM at 1 kHz rate and <10 kHz deviation

PHASE MODULATION (NOTE 4)
Display Ranges: 0 to .999 radians, 1 to 9.99 radians, 10 to 99.9 radians, 100 to 400 radians
Display Resolution: 3 digits

Maximum Deviation:

FREQUENCY BAND (MHz)	MAXIMUM DEVIATION (RADIANS)
0.01 to 15	50
15 to 32	12.5
32 to 64	25
64 to 128	50
128 to 256	100
256 to 512	200
512 to 1056	400

NOTE 4: *Phase Modulation specifications are valid where RF frequency - Mod frequency >150 kHz*

Table 1-1. Specifications for Model 6080A (cont.)

High-Rate Phase Modulation Maximum Deviation (Special Function 721):

FREQUENCY BAND (MHz)	MAXIMUM DEVIATION (RADIANS)
0.01 to 15	5
15 to 32	1.25
32 to 64	2.5
64 to 128	5
128 to 256	10
256 to 512	20
512 to 1056	40

Accuracy: ±(5% of setting + 0.1 radian) at 1 kHz rate
Distortion (NOTE 5): <2% THD from maximum deviation to to 1/2 max deviation, and <1% THD at 1/2 maximum deviation or less at 1 kHz rate.
3-dB Bandwidth: AC-coupled phase modulation, 20 Hz to 15 kHz
DC-coupled phase modulation, dc to 15 kHz
High-Rate Phase Modulation 3-dB Bandwidth (Special Function 721):
AC-coupled phase modulation, 20 Hz to 100 kHz
DC-coupled phase modulation, dc to 100 kHz
Incidental AM (valid for output frequency >500 kHz): 1% AM at 1 kHz rate for peak deviation <10 radians.

PULSE MODULATION (For RF Output Frequencies >10 MHz)
On/Off Ratio: 40 dB minimum for frequencies from 100 to 1056 MHz
60 dB minimum for frequencies <100 MHz
Rise and Fall Times: <15 ns, 10% to 90%
Level Error: For pulse widths >50 ns, the power in the pulse is within ±0.7 dB of the measured CW level.
Duty Cycle (External Modulation): 0 to 100%
Repetition Rate (External Modulation): DC to 10 MHz
Internal Modulation: Internal rates and widths
External Modulation: The pulse input is TTL compatible, terminated in 50Ω with internal active pull-up. It can be modeled as 1.2V in series with 50Ω at the pulse mod input connector. The instrument senses input terminal voltage and turns the RF OUTPUT off when the terminal voltage drops below 1±0.1V. The maximum allowable input is ±10V.

PULSE MODULATION (For RF Output Frequencies <10 MHz)
Rise and Fall Times: <2 times the period of the rf output frequency
Level Error: For pulse widths >10 times the period of the rf output frequency, the power in the pulse is within ±0.7 dB of the measured CW level.
Other pulse specifications are the same as for the >10 MHz frequency range.

NON-VOLATILE INSTRUMENT STATE MEMORY
50 instrument states are retained for typically 2 years, even with ac line power disconnected.

REVERSE-POWER PROTECTION
Protection Level: Up to 50 watts from a 50Ω source; up to 50V dc. RF OUTPUT is ac coupled. Protection is provided when the Signal Generator is turned off.

NOTE 5: *Valid for rates from 0.05 to 50 kHz in high-bandwidth mode. Does not include effects of residual phase noise.*

Table 1-1. Specifications for Model 6080A (cont.)

Trip/Reset: A flashing RF OFF annunciator indicates a tripped condition. Pushing RF ON/OFF button resets the Signal Generator.

IEEE-488 REMOTE CONTROL

Extent of Remote Control: All controls except the power switch and the internal/external reference switch are remotely programmable via the IEEE-488 Interface (Std. 488.2-1987). All status including the option complement are available remotely.

Interface Functions Supported: SH1, AH1, T5, TE0, L3, LE0, SR1, RL1, PP0, DC1, DT1, C0, and E2.

INTERNAL MODULATION SOURCE (Sine Wave)

Rates: 0.1 Hz to 200 kHz, key-selectable 400/1000 Hz

Display Ranges: 00.1 to 99.9 Hz
100 to 999 Hz
1.00 to 9.99 kHz
10.0 to 99.9 kHz
100 to 200 kHz

Frequency Resolution: 0.1 Hz or 3 digits

Frequency Accuracy: Same as reference oscillator ±7 millihertz

Output Level Range: 0 to 4V pk into 600Ω

Output Level Resolution: 1 mV pk or 3 digits, whichever is greater.

Distortion: <0.15% THD for output levels >0.2V pk and modulation frequency <20 kHz.

Output Level Accuracy: ±(4% + 15 mV) for modulation frequency <100 kHz.

Output Impedance: 600Ω ±2%

Other Waveforms Available by Special Function:

- Square Wave (Special Function 752)
- Triangle Wave (Special Function 751)
- Pulse (Special Functions 758,759), width 100 ns to 1/Fmod in 100 ns or 3-digit increments, whichever is greater. Rate and width are coherent with Signal Generator time base.

EXTERNAL MODULATION

1V pk provides indicated modulation index. Nominal input impedance is 600Ω. Maximum level is ±5V pk.

MODULATION MODES

Any combination of AM, PULSE, and FM or ØM, internal or external, may be used.

DIGITAL FREQUENCY SWEEP

Sweep Modes: Auto, single, or manual

Adjustable Parameters: Sweep symmetry, sweep speed, sweep width, and sweep increment.

Sweep Speed: Minimum 40 ms/increment selectable as (minimum + dwell time) where dwell time can be 0, 20, 50, 100, 200, or 500 ms at each increment.

DIGITAL AMPLITUDE SWEEP

Sweep Type: Linear (volts) or logarithmic (dB)

Sweep Modes: Auto, single, or manual.

ADJUSTABLE PARAMETERS: Sweep symmetry, sweep speed, sweep width, and sweep increment.

Sweep Speed: Minimum 30 ms/increment selectable as (minimum + dwell time) where dwell time can be 0, 20, 50, 100, 200, or 500 ms at each increment.

SWEEP OUTPUT (AUX Connector Pin 5)

0 to +10V±10%, up to 4096 points in a stepped ramp, load >2 kΩ.

Table 1-1. Specifications for Model 6080A (cont.)

PEN LIFT OUTPUT (AUX Connector Pin 4)

TTL level, high during sweep retrace, load >2 kΩ.

GENERAL SPECIFICATIONS

Temperature: Operating, 0 to +50°C (+32 to +122°F).
Non-Operating, -40 to +75°C (-40 to +167°F).

Operating Humidity Range: 95% to +30°C, 75% to +40°C, and 45% to +50°C.

Operating Altitude: Up to 10,000 ft.

Vibration: Non-operating, 5 to 15 Hz at 0.06 in, 15 to 25 Hz at 0.04 in, and 25 to 55 Hz at 0.02 in, double amplitude (DA).

Shock: Non-operating, bench handling per MIL T 28800C Class 5, Style E.

Electromagnetic Compatibility: The radiated emissions induce <0.5 μV (at rf carrier frequency) into a 1-inch diameter, 2-turn loop, 1-inch from any surface as measured into a 50Ω receiver.

Complies with Standards:

- CE03 of MIL-STD-461B (Power and interconnecting leads), 0.015 to 50 MHz.
- RE02 of MIL-STD-461B (14 kHz to 10 GHz).
- FCC Part 15, Class B.
- VDE 0871B
- CISPR 22

Size:	Width	Height	Depth
	43 cm	13.3 cm	59.7 cm
	17 in	5.25 in	23.5 in

Power Requirements: 100, 120, 220, or 240V, each ±10%; 48-63 Hz; 200 VA, <15 VA in standby, with any options installed.

Weight: 27 kg (60 lbs).

OPTION -130 HIGH-STABILITY REFERENCE

Aging Rate: <±5 x 10^{-10}/day, after 21 days continuous operation.

Temperature Stability: <±2 x 10^{-10}/°C. (Oven remains powered in standby.)

OPTION -132 MEDIUM-STABILITY REFERENCE

Aging Rate: <±1 x 10^{-7}/month after 5 days continuous operation.

Temperature Stability: <±1 x 10^{-7} (0 to +50°C)

OPTION -830 REAR PANEL CONNECTORS

Moves connectors for MODULATION INPUT, MOD output, and RF OUTPUT to the rear panel. The front panel connector locations are covered with plugs.

SUPPLEMENTAL CHARACTERISTICS

The following characteristics are provided to assist in Signal Generator applications, and to describe some other aspects of typical performance.

Frequency Switching Speed: <100 ms to settle within 100 Hz

Amplitude Switching Speed: <100 ms to settle within 0.1 dB

Pulse Modulation Delay: OFF to ON, 80 ns typical ON to OFF, 65 ns typical

Table 1-2. Specifications for Model 6082A

FREQUENCY

Range: 100 kHz to 2112 MHz. (See Internal Modulation Oscillator for coverage from 0.1 Hz to 200 kHz.)
Frequency Bands: The carrier frequency band endpoints are shown below.

BAND DESIGNATION	APPROXIMATE CARRIER FREQUENCY BAND (MHz)	SPECIFIC CARRIER FREQUENCY BAND (MHz)
A	0.1 to 15	0.1 to 14.999,999
B	15 to 32	15 to 31.999,999
C	32 to 64	32 to 63.999,999
D	64 to 128	64 to 127.999,999
E	128 to 256	128 to 255.999,999
F	256 to 512	256 to 511.999,999
G	512 to 1056	512 to 1055.999,999
H	1056 to 2112	1056 to 2112

Resolution: 1 Hz
Display Resolution: 10 digits
Stability: Same as Internal Reference Oscillator

10 MHz INTERNAL REFERENCE OSCILLATOR

Type: Temperature Compensated Crystal Oscillator (TCXO)
Temperature Stability: Less than ±1 ppm p-p over the range 0 to +50°C
Typical Aging Rate: Less than ±1 ppm/yr
Reference Output: 10 MHz, >0 dBm for 50Ω load, available at the rear-panel REF OUT connector.

PROVISION FOR EXTERNAL REFERENCE

The rear panel REF IN connector accepts an external source of 10 MHz ±10 ppm sine wave, 0.2 to 2.0V rms for a 50Ω load. One alternate external reference frequency setting of 1, 2, or 5 MHz is available at a time, through Special Function 761 or a remote command. The default alternate reference frequency is 5 MHz. See the Service Manual for setting internal DIP switches for use with a 1 or 2 MHz external reference.

AMPLITUDE

Range: +16 to -140 dBm for rf output frequency <1056 MHz.
+13 to -140 dBm for rf output frequency >1056 MHz.
Resolution: 0.1 dB (0.1% or 1 nV in volts). Annunciators for dB, dBm, V, mV, µV, dBf, dBµV, dBmV, and EMF
Display Resolution: 3 1/2 digits

Accuracy (+23 to ±5°C):

FREQUENCY (MHz)	AMPLITUDE IN dBm +16 +13 -127 -140
1.0 to 1056	±1 dBm
1056 to 2112	±1 dBm

Table 1-2. Specifications for Model 6082A (cont.)

Accuracy (0 to 50°C):

FREQUENCY (MHz)	AMPLITUDE IN dBm +16 to +13	+13 to -127	-127 to -140
0.1 to 0.4	±2 dBm	±2 dBm	±3 dBm
0.4 to 1056	±1.5 dBm	±1.5 dBm	±3 dBm
1056 to 2112	±1.5 dBm	±1.5 dBm	±3 dBm

Source SWR: <1.5:1 below +6 dBm
<2.0:1 above +6 dBm

Flatness (0 to 50°C): ±1.0 dB at +10 dBm

Intermodulation Distortion (Amplitude of +4 dBm, CW only):

FREQUENCY (MHz)	SPACING 1 kHz	25 kHz
0.1 to 128 MHz	-60 dBc	-80 dBc
128 to 512 MHz	-65 dBc	-75 dBc
512 to 2121 MHz	-65 dBc	-70 dBc

SPECTRAL PURITY (CW ONLY)

Spurious Signals: <-100 dBc for offsets greater than 10 kHz and rf output frequency <1056 MHz. <94 dBc for offsets greater than 10 kHz and rf output frequency >1056 MHz. Fixed-frequency spurious signals for rf output frequency <1056 MHz are <-100 dBc or <-140 dBm, whichever is greater. Fixed-frequency spurious signals for rf output frequency >1056 MHz are <-94 dBc or <-140 dBm, whichever is greater.

Harmonics: <-30 dBc for amplitudes less than +13 dBm at 1 to 2112 MHz.

Sub-harmonics: <-45 dBc for rf output frequencies from 1056 to 2112 MHz.

Power Line Spurious Signals (offsets less than 10 kHz): <-56 dBc for rf output frequencies <1056 MHz. <-50 dBc for rf output frequencies >1056 MHz.

Residual FM: (NOTE 1)

FREQUENCY BAND (MHz)	RESIDUAL FM 0.3 to 3 kHz	0.05 to 15 kHz
0.1 to 15	0.3	0.3
15 to 32	0.3	0.3
32 to 64	0.3	0.3
64 to 128	0.3	0.3
128 to 256	0.3	0.3
256 to 512	0.7	1.2
512 to 1056	1.5	2.5
1056 to 2112	3	5

NOTE 1: *Allowable operating modes CW, AM, FM (Peak dev. <1.5% of max in operating band), øM (same comment as FM), Pulse.*

Table 1-2. Specifications for Model 6082A (cont.)

SSB Phase Noise: (NOTE 1)

CARRIER FREQUENCY BAND (MHz)	OFFSET FREQUENCY 1 kHz (dBc/Hz)	20 kHz (dBc/Hz)	100 kHz (dBc/Hz)
0.1 to 15	-112	-138	-138
15 to 32	-124	-145	-146
32 to 64	-118	-144	-146
64 to 128	-112	-144	-145
128 to 256	-106	-141	-144
256 to 512	-100	-136	-142
512 to 1056	-94	-130	-138
1056 to 2112	-88	-124	-132

Residual AM (0.05 to 15 kHz Band): <-80 dBc (.01%)

AMPLITUDE MODULATION

Depth Range: 0% to 99.9% for rf output level <+7 dBm
AM Resolution: 0.1%
AM Display: 3 digits
AM Accuracy: ±(2% + 4% of setting) for rate = 1 kHz and depth <90%
AM Distortion (Rate = 1 kHz) (NOTE 2): <1.5% THD to 30% AM
<3% THD to 70% AM
<5% THD to 90% AM

AM 3-dB Bandwidth (NOTE 2): AC-coupled AM, 20 Hz to 50 kHz
DC-coupled AM, dc to 50 kHz

Incidental ØM: <0.20 radian for rates < 1 kHz and < 30% AM and frequencies <1056 MHz;
<0.40 radian for rates < 1 kHz and < 30% AM and frequencies >1056 MHz

FREQUENCY MODULATION (NOTE 3)

FM Display Ranges: 0 to 999 Hz
1 to 9.99 kHz
10 to 99.9 kHz
100 to 999 kHz
1 to 8.00 MHz
FM Display Resolution: 3 digits

NOTE 2: *AM specifications apply where RF output frequency - modulation frequency is greater than 150 kHz.*

NOTE 3: *FM specifications apply where: rf output frequency - deviation) >150 kHz, and rf output frequency - modulation rate >150 kHz.*

Table 1-2. Specifications for Model 6082A (cont.)

Maximum Deviation:

FREQUENCY BAND (MHz)	MAXIMUM DEVIATION	
	DC-COUPLED FM	AC-COUPLED FM (THE SMALLER OF)
0.1 to 15	500 kHz	500 kHz or fmod x 5,000
15 to 32	125 kHz	125 kHz or fmod x 1,250
32 to 64	250 kHz	250 kHz or fmod x 2,500
64 to 128	500 kHz	500 kHz or fmod x 5,000
128 to 256	1 MHz	1 MHz or fmod x 10,000
256 to 512	2 MHz	2 MHz or fmod x 20,000
512 to 1056	4 MHz	4 MHz or fmod x 40,000
1056 to 2112	8 MHz	8 MHz or fmod x 80,000

FM Distortion:

Standard Mode: <2% for 0.5 to 1.0 times maximum deviation; <1% for <0.5 times maximum deviation. Applies for rates of 50 Hz to 50 kHz.

Low-Distortion Mode (Special Function 731): <0.33% for <= 3.5 kHz peak deviation and rates 0.3 to 3 kHz.

FM Resolution: 3 digits.

FM Accuracy: ±(5% of setting + 10 Hz) for rates of 0.05 to 50 kHz

FM 3-dB Bandwidth:

DEVIATION	COUPLING	
	INTERNAL AC	EXTERNAL AC (DC)
0% to 25% Maximum	20 Hz to 175 kHz	20 Hz (dc) to 175 kHz
25% to 100% Maximum	20 Hz to 100 kHz	20 Hz (dc) to 100 kHz

Incidental AM: <1% depth for peak deviation <100 kHz at 1 kHz rate and carrier frequency >0.5 MHz

DC-Coupled FM Center Frequency Error, at 1 GHz, after dcFM internal cal, and without any FM range changes: <(.1% of dev + 500 Hz)

Low-Rate External AC-Coupled FM (Special Function 711):

FREQUENCY BAND (MHz)	MAX DEV, IN kHz (AT 10 Hz RATE)	
	SINE WAVE	SQUARE WAVE
0.1 to 15	80	40
15 to 32	20	10
32 to 64	40	20
64 to 128	80	40
128 to 256	160	80
256 to 512	320	160
512 to 1056	640	320
1056 to 2112	1280	640

Table 1-2. Specifications for Model 6082A (cont.)

Droop: <30% on a 5 Hz square wave
3-dB Bandwidth: 0.5 Hz to 100 kHz (typical)
Maximum dc Input: ±10 mV
Incidental AM: <1% AM at 1 kHz rate and <10 kHz deviation

PHASE MODULATION (NOTE 4)
Display Ranges: 0 to .999 radians
1 to 9.99 radians
10 to 99.9 radians
100 to 800 radians
Display Resolution: 3 digits
Maximum Deviation:

FREQUENCY BAND (MHz)	MAXIMUM DEVIATION (RADIANS)
0.1 to 15	50
15 to 32	12.5
32 to 64	25
64 to 128	50
128 to 256	100
256 to 512	200
512 to 1056	400
1056 to 2112	800

High-Rate Phase Modulation Maximum Deviation (Special Function 721):

FREQUENCY BAND (MHz)	MAXIMUM DEVIATION (RADIANS)
0.1 to 15	5
15 to 32	1.25
32 to 64	2.5
64 to 128	5
128 to 256	10
256 to 512	20
512 to 1056	40
1056 to 2112	80

Accuracy: ±(5% of setting + 0.1 radian) at 1 kHz rate
Distortion (NOTE 5): <2% THD from maximum deviation to to 1/2 max deviation, and <1% THD at 1/2 maximum deviation or less at 1 kHz rate.
3-dB Bandwidth: AC-coupled phase modulation, 20 Hz to 15 kHz
DC-coupled phase modulation, dc to 15 kHz

NOTE 4: *Phase Modulation specifications are valid where RF frequency - Mod frequency >150 kHz*
NOTE 5: *Valid for rates from 0.05 to 50 kHz in high-bandwidth mode. Does not include effects of residual phase noise.*

Table 1-2. Specifications for Model 6082A (cont.)

High-Rate Phase Modulation 3-dB Bandwidth (Special Function 721):
AC-coupled phase modulation, 20 Hz to 100 kHz
DC-coupled phase modulation, dc to 100 kHz
Incidental AM (valid for f >500 kHz): <1% AM at 1 kHz rate for peak deviation <10 radians.

PULSE MODULATION (For RF Output Frequencies >10 MHz)
On/Off Ratio: 80 dB minimum
Rise and Fall Times: <15 ns, 10% to 90%
Level Error: For pulse widths >50 ns, the power in the pulse is within ±0.7 dB of the measured CW level.
Duty Cycle (External Modulation): 0 to 100%
Repetition Rate (External Modulation): DC to 10 MHz
Internal Modulation: Internal rates and widths
External Modulation: The pulse input is TTL compatible, terminated in 50Ω with internal active pull-up. It can be modeled as 1.2V in series with 50Ω at the pulse mod input connector. The instrument senses input terminal voltage and turns the RF OUTPUT off when the terminal voltage drops below 1±0.1V. The maximum allowable input is ±10V.

PULSE MODULATION (For RF Output Frequencies <10 MHz)
Rise and Fall Times: <2 times the period of the rf output frequency
Level Error: For pulse widths >10 times the period of the rf output frequency, the power in the pulse is within ±0.7 dB of the measured CW level.
Other pulse specifications are the same as for the >10 MHz frequency range.

NON-VOLATILE INSTRUMENT STATE MEMORY
50 instrument states are retained for typically 2 years, even with ac line power disconnected.

REVERSE-POWER PROTECTION
Protection Level: Up to 25 watts from a 50Ω source; up to 25V dc. RF OUTPUT is ac coupled. Protection is provided when the Signal Generator is turned off.
Trip/Reset: A flashing RF OFF annunciator indicates a tripped condition. Pushing RF ON/OFF button resets the Signal Generator.

IEEE-488 REMOTE CONTROL
Extent of Remote Control: All controls except the power switch and the internal/external reference switch are remotely programmable via the IEEE-488 Interface (Std. 488.2-1987). All status including the option complement are available remotely.
Interface Functions Supported: SH1, AH1, T5, TE0, L3, LE0, SR1, RL1, PP0, DC1, DT1, C0, and E2.

INTERNAL MODULATION SOURCE (Sine Wave)
Rates: 0.1 Hz to 200 kHz, key-selectable 400/1000 Hz
Display Ranges: 00.1 to 99.9 Hz
100 to 999 Hz
1.00 to 9.99 kHz
10.0 to 99.9 kHz
100 to 200 kHz
Frequency Resolution: 0.1 Hz or 3 digits
Frequency Accuracy: Same as reference oscillator ±7 millihertz

Table 1-2. Specifications for Model 6082A (cont.)

Output Level Range: 0 to 4V pk into 600Ω
Output Level Resolution: 1 mV pk or 3 digits, whichever is greater.
Distortion: <0.15% THD for output levels >0.2V pk and modulation frequency <20 kHz.
Output Level Accuracy: ±(4% + 15 mV) for modulation frequency <100 kHz.
Output Impedance: 600Ω ±2%
Other Waveforms Available by Special Function:
- Square Wave (Special Function 752)
- Triangle Wave (Special Function 751)
- Pulse (Special Functions 758,759), width 100 ns to 1/Fmod in 100 ns or 3-digit increments, whichever is greater. Rate and width are coherent with Signal Generator time base.

EXTERNAL MODULATION

1V pk provides indicated modulation index. Nominal input impedance is 600Ω. Maximum level is ±5V pk.

MODULATION MODES

Any combination of AM, PULSE, and FM or ØM, internal or external, may be used.

DIGITAL FREQUENCY SWEEP

Sweep Modes: Auto, single, or manual
Adjustable Parameters: Sweep symmetry, sweep speed, sweep width, and sweep increment.
Sweep Speed: Minimum 40 ms/increment selectable as (minimum + dwell time) where dwell time can be 0, 20, 50, 100, 200, or 500 ms at each increment.

DIGITAL AMPLITUDE SWEEP

Sweep Type: Linear (volts) or logarithmic (dB)
Sweep Modes: Auto, single, or manual.
Adjustable Parameters: Sweep symmetry, sweep speed, sweep width, and sweep increment.
Sweep Speed: Minimum 30 ms/increment selectable as (minimum + dwell time) where dwell time can be 0, 20, 50, 100, 200, or 500 ms at each increment.

SWEEP OUTPUT (AUX Connector Pin 5)

0 to +10V±10%, up to 4096 points in a stepped ramp, load >2 kΩ.

PEN LIFT OUTPUT (AUX Connector Pin 4)

TTL level, high during sweep retrace, load >2 kΩ.

GENERAL SPECIFICATIONS

Temperature: Operating, 0 to +50°C (+32 to +122°F).
Non-Operating, -40 to +75°C (-40 to +167°F).
Operating Humidity Range: 95% to +30°C, 75% to +40°C, and 45% to +50°C.
Operating Altitude: Up to 10,000 ft.
Vibration: Non-operating, 5 to 15 Hz at 0.06 in, 15 to 25 Hz at 0.04 in, and 25 to 55 Hz at 0.02 in, double amplitude (DA).
Shock: Non-operating, bench handling per MIL T 28800C Class 5, Style E.
Electromagnetic Compatibility: The radiated emissions induce <0.5 µV (at rf carrier frequency) into a 1-inch diameter, 2-turn loop, 1-inch from any surface as measured into a 50Ω receiver.

Table 1-2. Specifications for Model 6082A (cont.)

Complies with Standards:

- CE03 of MIL-STD-461B (Power and interconnecting leads), 0.015 to 50 MHz.
- RE02 of MIL-STD-461B (14 kHz to 10 GHz).
- FCC Part 15, Class B.
- VDE 0871B
- CISPR 22

Size:	Width	Height	Depth
	43 cm	13.3 cm	59.7 cm
	17 in	5.25 in	23.5 in

Power Requirements: 100, 120, 220, or 240V, each ±10%; 48-63 Hz; 200 VA, <15 VA in standby, with any options installed.

Weight: 27 kg (60 lbs).

OPTION -130 HIGH-STABILITY REFERENCE

Aging Rate: $<\pm 5 \times 10^{-10}$/day, after 21 days continuous operation.

Temperature Stability: $<\pm 2 \times 10^{-10}$/°C. (Oven remains powered in standby.)

OPTION -132 MEDIUM-STABILITY REFERENCE

Aging Rate: $<\pm 1 \times 10^{-7}$/month after 5 days continuous operation.

Temperature Stability: $<\pm 1 \times 10^{-7}$ (0 to +50°C)

OPTION -830 REAR PANEL CONNECTORS

Moves connectors for MODULATION INPUT, MOD output, and RF OUTPUT to the rear panel. The front panel connector locations are covered with plugs.

SUPPLEMENTAL CHARACTERISTICS

The following characteristics are provided to assist in Signal Generator applications, and to describe some other aspects of typical performance.

Frequency Switching Speed: <100 ms to settle within 100 Hz

Amplitude Switching Speed: <100 ms to settle within 0.1 dB

Pulse Modulation Delay: OFF to ON, 80 ns typical ON to OFF, 65 ns typical

Section 2
Installation

INTRODUCTION 2-1.

This section provides instructions for unpacking and installing the Signal Generator. Procedures for selecting line voltage, replacing the fuse, rack mounting, and configuration of the Signal Generator for local and remote operation are provided here.

UNPACKING AND INSPECTION 2-2.

The Signal Generator is shipped in a special protective carton that should prevent damage during shipment. Check the shipping order against the contents of the carton and report any damage or short shipment to the place of purchase or the nearest Fluke Technical Service Center. Instructions for inspection and claims are included on the shipping container. Refer to Section 1 for reshipment instructions.

The shipping container should include the items in Table 2-1. Accessories ordered for the Signal Generator are shipped in a separate container. Table 2-2 lists accessories available for the Signal Generator.

RACK OR BENCH MOUNTING 2-3.

CAUTION

To prevent overheating, allow at least 3 inches of clearance behind and on each side of the Signal Generator.

The Signal Generator may be placed directly on a work bench or mounted in a standard (24-inch deep) equipment rack. Use the Fluke Y6001 Rack Mount Kit for mounting the Signal Generator in an equipment rack. Instructions for installing the Signal Generator with the Rack Mount Kit are provided in the kit. The outside dimensions of the Signal Generator are shown in Table 1-1. The Rack Mount Kit is comprised of a 5 ¼-inch Rack Adapter (PN M05-205-600) and 24-inch Rack Slides (PN M00-280-610).

POWER REQUIREMENTS 2-4.

The Signal Generator uses a line voltage of 110/120V ac ±10%, with a 2.0A fast-blow fuse; or 220/240V ac ±10%, with a 1.0A fast-blow fuse. The line frequency must be between 48 and 63 Hz. Power consumption of the Signal Generator is less than 200 VA.

Table 2-1. Standard Equipment

ITEM	MODEL OR PART NUMBER
Signal Generator	6080A or 6082A
Line Power Cord	See Table 2-2 and Figure 2-1
6080A/82A Operator Manual	861034
6080A/82A Operator Reference Guide	882154
6080A/82A Remote Programming Reference Guide	882147
6080A/82A Special Functions Decal	860911
6080A Service Manual	868914
or	
6082A Service Manual	881888
Two BNC dust caps	478982

Table 2-2. Line Power Cord Types Available from Fluke

TYPE	VOLTAGE/CURRENT	FLUKE OPTION NUMBER
North America	120V/15A	LC-1
North America	240V/15A	LC-2
Universal Euro	220V/16A	LC-3
United Kingdom	240V/13A	LC-4
Switzerland	220V/10A	LC-5
Australia	240V/10A	LC-6
South Africa	240V/5A	LC-7

LINE VOLTAGE SELECTION AND FUSE REPLACEMENT 2-5.

CAUTION

To prevent instrument damage, verify that the correct fuse is installed for the line voltage setting, and that the line voltage setting is compatible with local line power before plugging in the line cord.

The Signal Generator arrives from the factory configured for the line voltage normally appropriate for the country of purchase, or as specified at the time of your purchase order. The Signal Generator also comes with the appropriate line power plug for the country of purchase. If you need a different type, refer to Table 2-3 and Figure 2-1. They list and illustrate the line power plug types available from Fluke.

Refer to Figure 2-2 to set the line voltage of the Signal Generator to match the available source. Insert the small pc board in the fuse module so that the appropriate voltage label is towards you. Figure 2-2 also shows how to replace the line fuse. A plate attached to the rear panel shows the correct fuse value for each of the two line voltages.

Table 2-3. Accessories

DESCRIPTION	ACCESSORY NO.
Rack Mount Kit Includes M05-205-600 (5 1/4-inch Rack Mount Ears) and M00-280-610 (24-inch Rack Slides)	Y6001
IEEE-488 Shielded Cable, 1 meter	Y8021
IEEE-488 Shielded Cable, 2 meters	Y8022
IEEE-488 Shielded Cable, 4 meters	Y8023
Coaxial Cable, 50 ohms, 3 feet, BNC (m) both ends	Y9111
Coaxial Cable, 50 ohms, 6 feet, BNC (m) both ends	Y9112

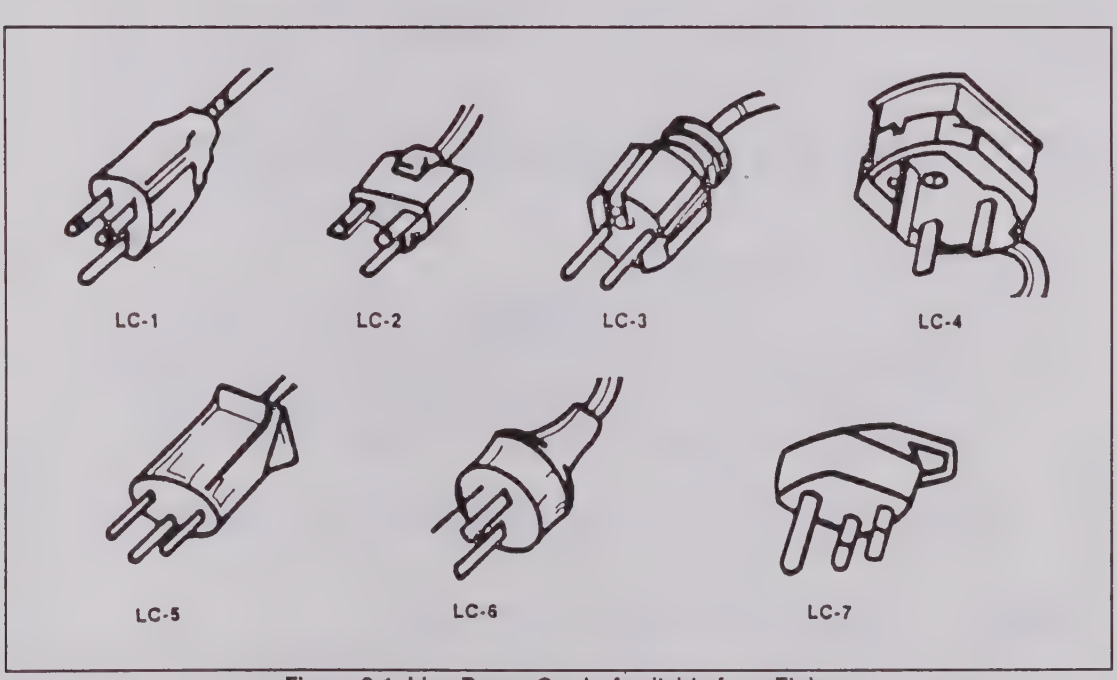

Figure 2-1. Line Power Cords Available from Fluke

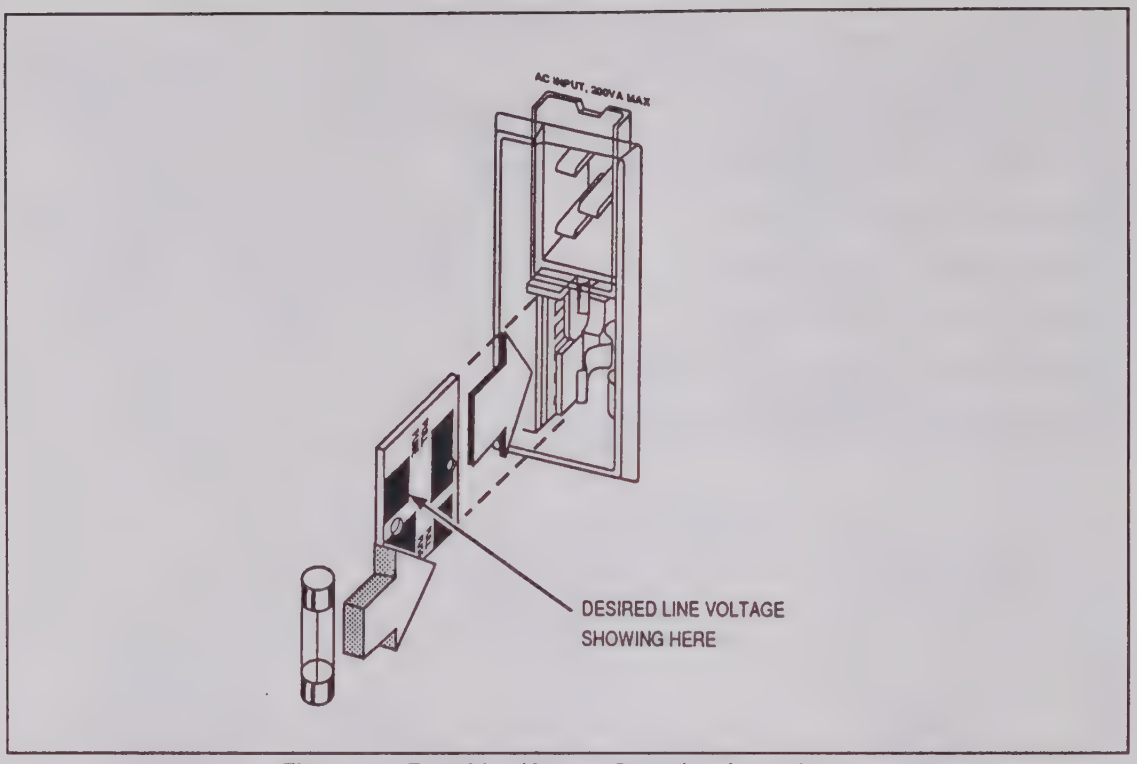

Figure 2-2. Fuse/Line Voltage Selection Assembly

CONNECTING TO LINE POWER 2-6.

WARNING

TO AVOID SHOCK HAZARD, CONNECT THE FACTORY SUPPLIED THREE-CONDUCTOR LINE POWER CORD TO A PROPERLY GROUNDED POWER OUTLET. DO NOT USE A TWO-CONDUCTOR ADAPTER OR EXTENSION CORD; THIS WILL BREAK THE PROTECTIVE GROUND CONNECTION.

After you verify that the line voltage selection pc board is in the correct position, verify that the correct fuse for that line voltage is installed. Connect the Signal Generator to a properly grounded three-prong outlet.

INTERNAL/EXTERNAL FREQUENCY REFERENCE 2-7.

The Signal Generator normally operates with an internal reference oscillator. However, if desired, the Signal Generator can be operated with an external reference by setting the rear panel REF INT/EXT switch to EXT and connecting the external reference to the REF IN connector.

NOTE

When the Signal Generator is operating on internal reference, a 10-MHz Signal is present at the 10 MHz OUT connector. To meet the specified radiated emissions, this connector must be terminated with a BNC non-shorting dust cap. A dust cap, PN 478982, is supplied with the signal Generator. If a cable is connected, it must be a double-shielded coaxial cable such as RG-223 terminated in a 50-ohm load.

NOTE

Do not operate the Signal Generator on internal reference with an external reference signal applied. This causes output spectral degradation.

LOCAL AND REMOTE OPERATION 2-8.

The Signal Generator output is controlled by either local (front panel) operation or remote operation. in the local operation mode, controls on the front panel are used to control the Signal Generator. In Remote, an IEEE-488 controller controls the Signal Generator by sending programming commands over the IEEE-488 Interface. Section 5 provides instructions for remote operation.

NOTE

To meet the specified radiated emissions, a shielded IEEE-488 cable, such as a Fluke Y8021 must be used.

POWER-ON SEQUENCE 2-9.

When the Signal Generator is turned on, a power-on sequence starts. During the power-on sequence, the microprocessor tests the front panel display, the analog circuitry, the instrument RAM, and the nonvolatile memory containing compensation and calibration data. A front panel display test lights all segments for a brief period while the rest of the self-tests take place. After succesful completion of the self tests, the Signal Generator is in the preset state, as defined in Appendix A. The instrument settings in effect when the Signal Generator was turned off can be recalled by pressing [RCL] [0] [0].

If any of the self-tests fail, the Signal Generator displays one or more status codes. Any front panel entry that occurs before the power-on sequence is completed aborts the self-test, and sets the Signal Generator to the preset state. The power-on self-tests are explained in detail in the Service Manual.

Section 3
Features

INTRODUCTION 3-1.

Section 3 is a reference for the functions and locations of the front panel and rear panel features of the Signal Generator. Please read this information before operating the Signal Generator. Front panel operating instructions are provided in Section 4, and remote operating instructions are provided in Section 5.

FRONT PANEL FEATURES 3-2.

Figure 3-1 shows the front panel. Table 3-1 describes the front panel features.

REAR PANEL FEATURES 3-3.

Figure 3-2 shows the rear panel. Table 3-3 describes the rear panel features.

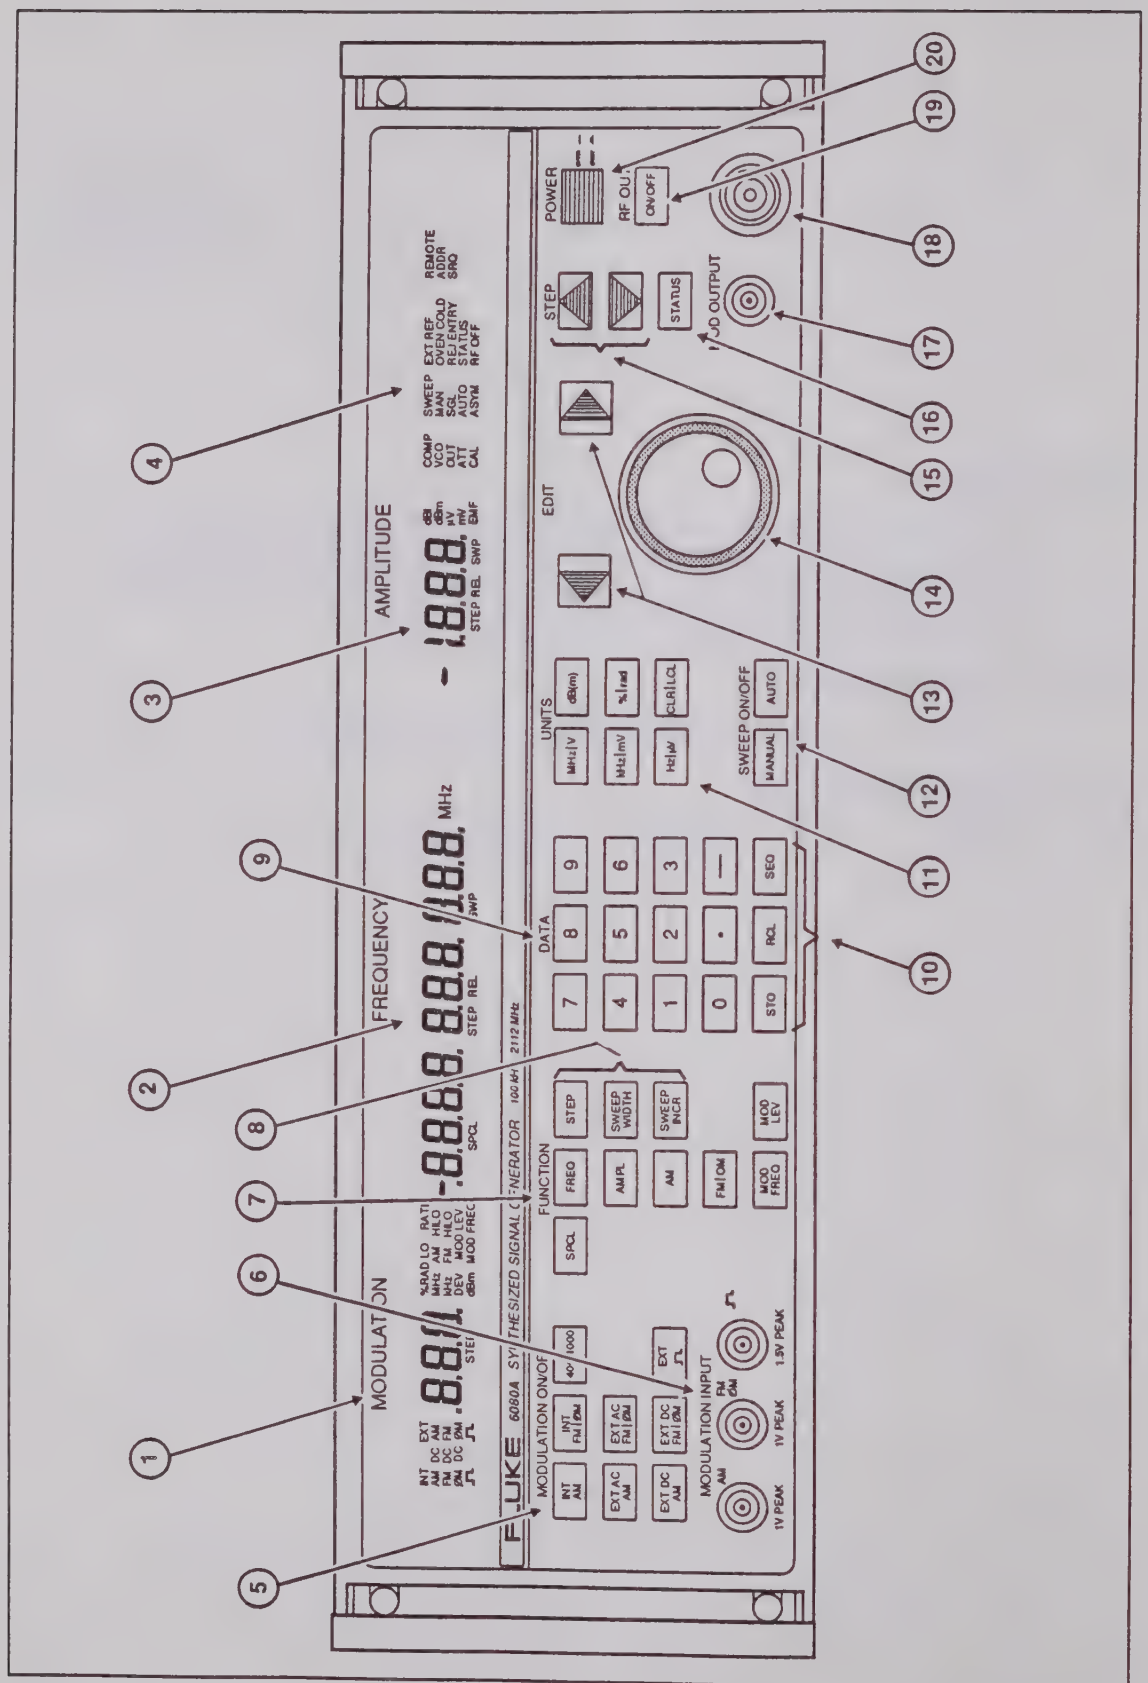

Figure 3-1. Front Panel Features

Table 3-1. Front Panel Features

①	**MODULATION DISPLAY FIELD**	A three-digit display, with associated annunciators, used to display the AM depth, FM/ØM deviation, source of modulation signal, modulation frequency and modulation level. It is also used to display active error codes and status codes.
	INT AM	Indicates that the internal modulation oscillator signal is amplitude modulating the output.
	INT FM	Indicates that the internal modulation oscillator signal is frequency modulating the output.
	INT ØM	Indicates that the internal modulation oscillator signal is phase modulating the output.
	INT ⎍	Indicates that the internal modulation oscillator signal is pulse modulating the output.
	EXT AC	Indicates that the ac-coupled signal at the AM MODULATION INPUT connector is amplitude modulating the output.
	EXT DC AM	Indicates that the dc-coupled signal at the AM MODULATION INPUT connector is amplitude modulating the output.
	EXT DC FM	Indicates that the dc-coupled signal at the FM/ØM MODULATION INPUT connector is frequency modulating the output.
	EXT FM	Indicates that the ac-coupled signal at the FM/ØM MODULATION INPUT connector is frequency modulating the output.
	EXT ØM	Indicates that the ac-coupled signal at the FM/ØM MODULATION INPUT connector is phase modulating the output.
	EXT DC ØM	Indicates that the dc-coupled signal at the FM/ØM MODULATION INPUT connector is phase modulating the output.
	EXT ⎍	Indicates that the dc-coupled signal at the FM/ØM MODULATION INPUT connector is pulse modulating the output.
	STEP	Indicates that the Step Size Entry, and Step Increment and Decrement keys affect the displayed modulation parameter.
	%	Indicates that the value displayed is the AM depth in percent.
	MHz kHz DEV	Indicates that the value displayed is the FM deviation in MHz, kHz, or Hz.
	rad	Indicates that the value displayed is the Phase Modulation Deviation in radians.
	dBm	Indicates that the value displayed is the target level in dBm when performing a level calibration/compensation procedure.

Table 3-1. Front Panel Features (cont)

	LO RATE	Indicates that the Signal Generator is in low-rate FM modulation mode.
	AM HI	Indicates that the external ac-coupled AM modulation signal is more than 2% above the nominal 1V pk input requirement.
	AM LO	Indicates that the external ac-coupled AM modulation signal is more than 2% below the nominal 1V pk input requirement.
	FM HI	Indicates that the external ac-coupled FM modulation signal is more than 2% above the nominal 1V pk input requirement.
	FM LO	Indicates that the external ac-coupled FM modulation signal is more than 2% below the nominal 1V pk input requirement.
	V MOD LEV	Indicates that the value displayed is the peak modulation output Level in volts.
	Hz kHz MOD FREQ	Indicates that the value displayed is the modulation frequency in Hz or kHz.
(2)	**FREQUENCY DISPLAY FIELD**	A signed 10-digit display with four annunciators that displays rf output frequency parameters of the Signal Generator. It is also used to display Special Function codes, status codes, or stored/recalled memory location codes.
	STEP	Indicates that the Step Size Entry and the Step Increment and Decrement keys affect the rf frequency.
	REL	Indicates that the displayed frequency is relative to a reference frequency.
	SPCL	Indicates certain Special Functions are enabled that are not otherwise annunciated. Pressing the [SPCL] key causes the enabled Special Function codes to be displayed.
	SWP	Indicates that the SWEEP ON/OFF keys apply to frequency sweep.
(3)	**AMPLITUDE DISPLAY FIELD**	A signed 3 1/2-digit display with eight annunciators that displays rf output amplitude parameters and status codes. Except when EMF units are selected, displayed amplitudes are referenced to a 50Ω load.
	STEP	Indicates that the Step Size Entry and the Step Increment and Decrement keys affect the rf output amplitude.
	REL	Indicates that the displayed amplitude is relative to a reference amplitude.
	SWP	Indicates that the SWEEP ON/OFF keys apply to amplitude sweep.

Table 3-1. Front Panel Features (cont)

	dBf	Indicates that the displayed amplitude is in decibels relative to one femtowatt.
	dB	Indicates that the displayed amplitude is in decibels relative to a reference amplitude, or is a step size value, a sweep increment value, or a sweep width value.
	dBm	Indicates that the displayed amplitude is in decibels relative to one milliwatt.
	V µV mV	Indicates that the displayed amplitude is in volts, microvolts, or millivolts.
	dB mV	Indicates that the displayed amplitude is in decibels relative to one millivolt.
	dB µV	Indicates that the displayed amplitude is in decibels relative to one microvolt.
	EMF	Indicates that the displayed amplitude is in EMF units, delivered into an open circuit or unterminated output. Toggled by Special Function 851/850.
(4)	**STATUS DISPLAY ANNUNCIATORS**	The status display field is composed of 17 annunciators and a yellow LED, all of which denote the status of the Signal Generator.
	COMP	Indicates that a compensation procedure is in progress. Flashes when the rear panel CAL|COMP switch is set to 1 (ON).
	VCO	Indicates that a coarse loop, sum loop, or subsynthesizer compensation procedure is in progress.
	OUT	Indicates that an output compensation procedure is in progress.
	ATT	Indicates that an attenuator compensation procedure is in progress.
	CAL	Indicates that a calibration procedure is in progress. Flashes when the rear panel CAL|COMP switch is set to 1 (ON).
	SWEEP	Indicates that a sweep is active.
	MAN	Indicates that manual sweep mode is active.
	SGL	Indicates that single sweep mode is active.
	AUTO	Indicates that auto sweep mode is active.

Table 3-1. Front Panel Features (cont)

	ASYM	Indicates that the Signal Generator is configured to sweep in asymmetric mode.
	EXT REF	Indicates that the rear panel REF switch is in the EXT (external) position.
	OVEN COLD	Indicates ovened timebase oscillator has not stabilized.
	REJ ENTRY	Flashes when an invalid entry is made.
	STATUS	Indicates when the Signal Generator is operating outside its specified range. Flashes when a hardware-limited or a hardware fault condition is detected.
	RF OFF	Indicates that the RF OUTPUT is disabled. Flashes when the RPP has been tripped.
	REMOTE	Indicates that the Signal Generator is in the remote (IEEE-488 Interface) mode of operation.
	ADDR	Indicates that the Signal Generator is addressed to listen or talk on the IEEE-488 interface Bus.
	SRQ	Indicates that the Signal Generator has asserted the IEEE-488 SRQ signal.
	Yellow LED	When lit, indicates that the Signal Generator is in the standby state and is connected to the power mains. The LED is off when the Signal Generator is operating.
(5)	**MODULATION ON/OFF KEYS**	Used to select type and source of modulation. With the exception of the [400/1000] key, these keys operate as independent push-on/push-off switches for the given modulation.
	[INT AM]	Enables internal amplitude modulation.
	[EXT AC AM]	Enables external ac-coupled amplitude modulation using the signal applied to the AM MODULATION INPUT connector.
	[EXT DC AM]	Enables external dc-coupled amplitude modulation using the signal applied to the AM MODULATION INPUT connector.
	[INT FM/ØM]	Enables internal frequency or phase modulation.
	[EXT AC FM/ØM]	Enables external ac-coupled frequency or phase modulation using the signal applied to the FM/ØM MODULATION INPUT connector.
	[EXT DC FM/ØM]	Enables external dc frequency or phase modulation using the signal applied to the FM/ØM MODULATION INPUT connector.
	[400/1000]	Toggles the internal modulation oscillator frequency between 400 and 1000 Hz. Used as an alternative to the [MOD FREQ] key and data input.

Table 3-1. Front Panel Features (cont)

	EXT ⎍	Enables external pulse modulation using the signal applied to the ⎍ MODULATION INPUT connector.
⑥	**MODULATION INPUT CONNECTORS**	
	AM	A BNC connector for input of a 1V pk external AM modulation signal.
	FM/ØM	A BNC connector for input of a 1V pk external FM/ØM modulation signal.
	⎍	A BNC connector for input of a 1.5V pk external pulse modulation signal.
⑦	**FUNCTION KEYS**	These keys are used to select a function parameter to be entered or edited. When pressed, the bright digit appears in the corresponding display field of the selected function.
	SPCL	Enables the Special Function mode. Special functions are enabled and disabled by using the DATA keys to enter a two-or-three digit numeric code. Refer to Section 4F, "Special Functions" for a detailed description and a list of the special functions.
	FREQ	Selects the rf output frequency parameter to be programmed.
	AMPL	Selects the rf output amplitude parameter to be programmed.
	AM	Selects the amplitude modulation depth parameter to be programmed.
	FM/ØM	Selects the frequency or phase modulation deviation parameter to be programmed.
	MOD FREQ	Selects the modulation frequency parameter to be programmed.
	MOD LEV	Selects the modulation level parameter to be programmed.
⑧	**FUNCTION MODIFIER KEYS**	
	STEP	After selecting one of the six functions, pressing this key displays the step size for the parameter and allows a new step size to be entered. The STEP △ or ▽ (increase or decrease) keys are enabled for the selected parameter.
	SWEEP WIDTH	After the frequency or amplitude function has been selected, pressing this key displays the sweep width for the function and allows a new sweep width to be entered. The SWEEP mode keys are enabled for the selected function.

Table 3-1. Front Panel Features (cont)

	SWEEP INCR	After the frequency or amplitude function has been selected, pressing this key displays the sweep increment for the function and allows a new sweep increment to be entered. The SWEEP mode keys are enabled for the selected function.
(9)	**DATA**	A 10-digit (plus sign and decimal key) keypad used for entering a parameter value, a Special Function code, or an Instrument State Memory recall/store location.
(10)	**INSTRUMENT STATE MEMORY OPERATION KEYS**	
	STO	Used with the DATA keys to store the current instrument state in a memory location. Memory locations 01 through 50 are available. You can store a single function parameter when you use one of these keys with any of the six FUNCTION keys.
	RCL	Used with the DATA keys to recall an instrument state from a memory location. Memory locations 01 through 50 are available for storage of instrument states. (Location 00 retains the instrument state in effect when the power is turned off and location 98 contains the Instrument Preset State described in Appendix A.) You can recall a single function parameter when you use one of these keys with any of the six FUNCTION keys.
	SEQ	Sequentially recalls, in increasing location order, the instrument state stored in memory. While the SEQ key is pressed, successive memory locations are displayed. When the key is released, the location last displayed is recalled. Pressing RCL followed by — sequentially recalls, in decreasing order, the stored instrument states.
(11)	**UNITS KEYS**	These keys, with the exception of CLR/LCL, terminate entry of a function parameter. You can also use these keys to convert displayed amplitude or FM/ØM units.
	MHz/V	Used with the FREQ, FM/ØM, and MOD FREQ function keys to specify units of megahertz. Used with the AMPL and MOD LEV function keys to specify units of volts. You also use this key with the Pulse Width Entry Special Function to specify units of microseconds.
	kHz/mV	Used with the FREQ, FM/ØM, and MOD FREQ function keys to specify units of kilohertz. You also use this key with the AMPL and MOD LEV function keys to specify units of millivolts, and with the Pulse Width entry Special Function to specify units of milliseconds.
	Hz/µV	Used with the FREQ, FM/ØM, and MOD FREQ function keys to specify units of hertz. Used with the AMPL and MOD LEV function keys to program the parameter data in units of microvolts. Used with the Pulse Width entry Special Function to program the parameter data in units of seconds.

Table 3-1. Front Panel Features (cont)

	dB(m)	Used with the AMPL function key to program the parameter data in terms of decibels relative to one milliwatt or to an alternate reference if selected by Special Function. You also use this key in relative amplitude mode or with the STEP SWEEP WIDTH or SWEEP INCR function modifier keys to specify units of decibels ratio.
	%/rad	Used with the AM function key to program the parameter data in units of percentage of AM depth. You also use this key with the FM/ØM function key to specify units of radians of ØM deviation.
	CLR/LCL	When the Signal Generator is in local operation, this key clears an entry and returns the Signal Generator to the last valid state. When the Signal Generator is in remote operation, this key returns local control.
(12)	**SWEEP ON/OFF KEYS**	These keys enable or disable a sweep mode. The keys operate as independent push-on and push-off switches for the given sweep mode.
	MANUAL	Enable or disable manual sweep mode. The edit knob is used to move up or down within the sweep range for the selected sweep function.
	AUTO	Enable or disable auto sweep mode. The Signal Generator repetitively progresses through the sweep range for the selected sweep function.
(13)	**EDIT KEYS**	These keys position the bright digit within a display field. Both keys repeat while they are pressed.
	◁	Moves the bright digit one digit to the left in the active display field.
	▷	Moves the bright digit one digit to the right in the active display field.
(14)	**EDIT KNOB**	Used to increase or decrease the value of the bright digit. You move the bright digit to the desired display field by pressing the one of the FUNCTION keys.
(15)	**STEP KEYS**	These two keys work in conjunction with the STEP Function Modifier key. Both keys repeat while held down.
	△	Increments the function parameter for the field that has has STEP annunciator lit, by the programmed step size.
	▽	Decrements the function parameter for the field that has has STEP annunciator lit, by the programmed step size.
(16)	**STATUS KEY**	Used to display a Rejected Entry (REJ ENTRY annunciator flashing) or Status codes in the display fields.
(17)	**MOD OUTPUT CONNECTOR**	A BNC connector for output of the internal modulation oscillator signal.

Table 3-1. Front Panel Features (cont)

(18)	**RF OUTPUT CONNECTOR**	A Type "N" connector that supplies the Signal Generator rf output signal.
(19)	**RF OUTPUT KEY**	A push-on/push-off key (with a corresponding RF OFF ON/OFF annunciator in the STATUS display field) that enables and disables the rf output of the Signal Generator.
(20)	**POWER SWITCH**	A push-on/push-to-standby detent switch that enables line power to the Signal Generator or enables standby power.

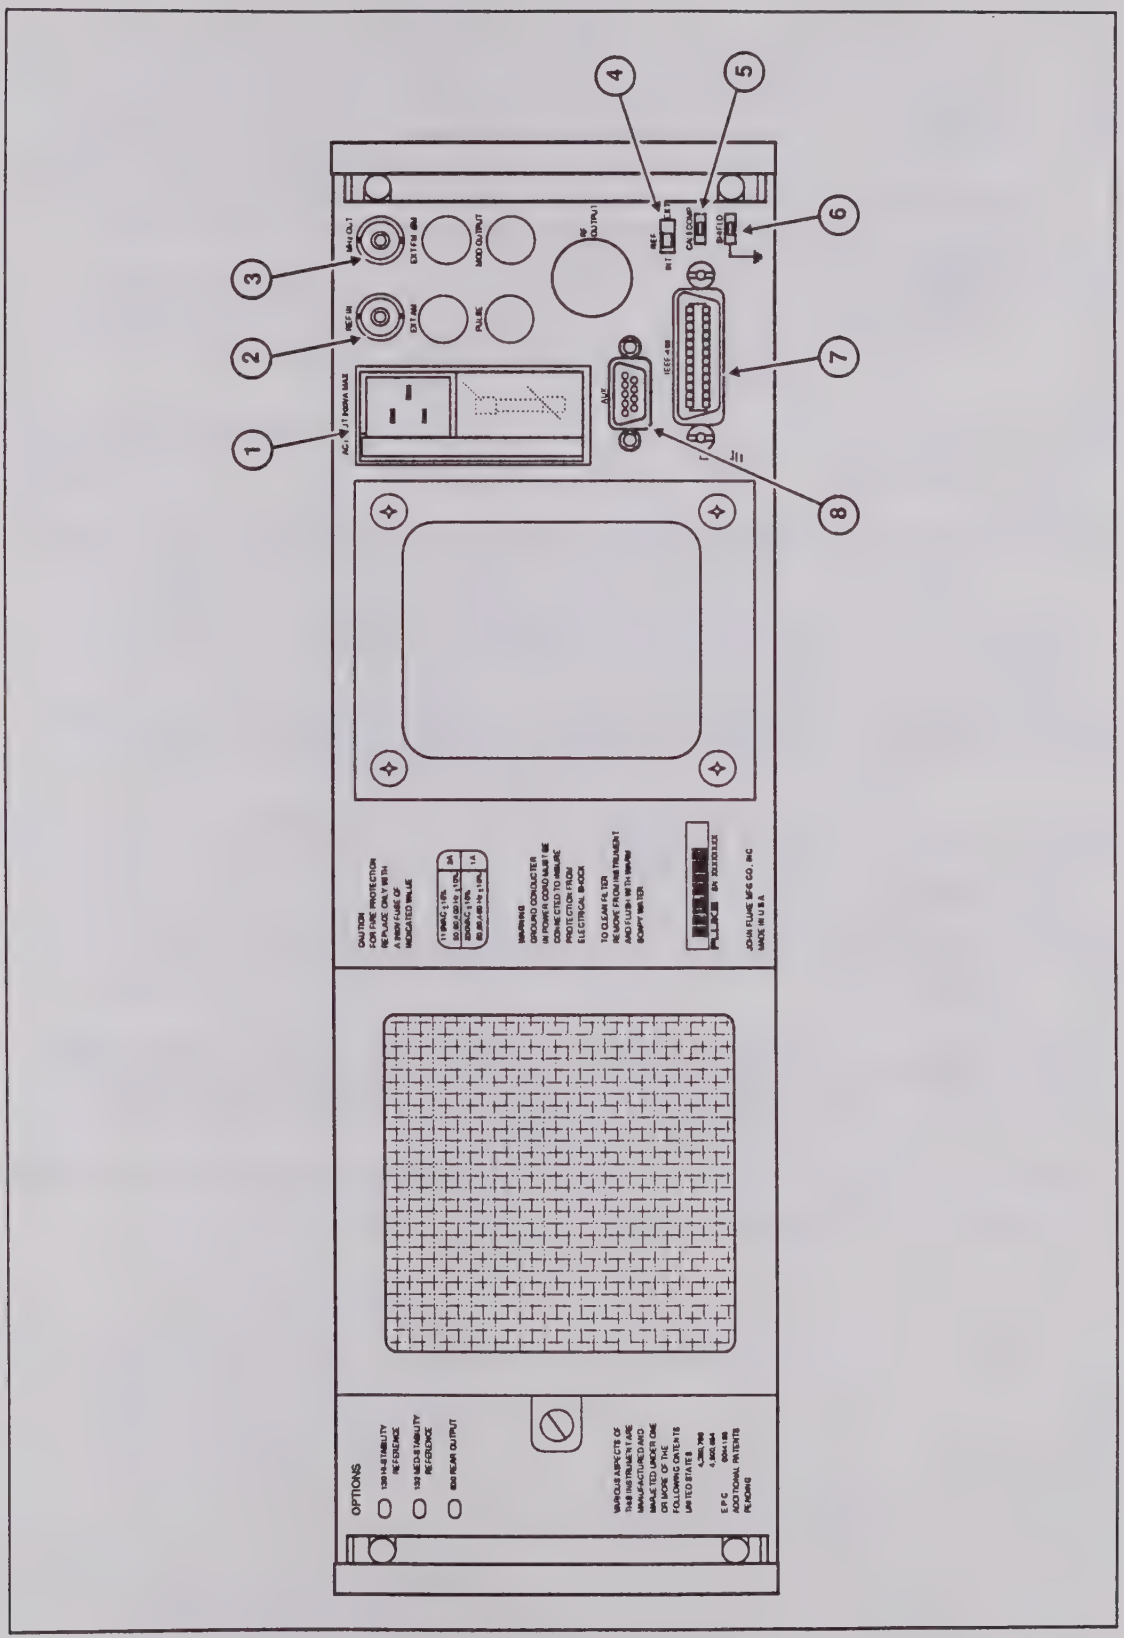

Figure 3-2. Rear Panel Features

Table 3-2. Rear Panel Features

①	**AC INPUT MODULE**	Permits operation from 115V or 230V. The number visible through the window on the selector card indicates the nominal line voltage to which the Signal Generator must be connected. The line voltage is selected by orienting the selector card appropriately. A 2-ampere fuse is required for 115V operation and a 1-ampere fuse is required for 230V operation.
②	**REF IN CONNECTOR**	A BNC connector that accepts a 1 MHz, 2 MHz, 5 MHz, or 10 MHz, 0.2 to 2V rms sine or square wave signal into a nominal 50Ω termination. This becomes the Signal Generator reference signal when the REF INT/EXT switch is set to EXT.
③	**10 MHz OUT CONNECTOR**	A BNC connector that presents a 10 MHz reference signal, greater than 0 dBm for a 50Ω load, to external devices.
④	**REF INT/EXT SWITCH**	This switch selects the Signal Generator frequency reference. When set to INT, the Signal Generator operates on the 10-MHz internal reference. The internal 10 MHz reference signal is available at the 10-MHz OUT connector. When set to EXT, the Signal Generator reference is a 1, 2, 5 or 10-MHz signal applied to the external REF IN connector.
⑤	**CALCOMP SWITCH**	When set to 1, enables the Signal Generator to run closed-case calibration and compensation procedures. When set to 0, it write-protects calibration and compensation data memory.
⑥	**Shield ⏚ SWITCH**	This switch connects the shield of the IEEE-488 connector and cable to the instrument ground.
⑦	**IEEE-488 CONNECTOR**	Allows remote operation of the Signal Generator via the IEEE-488 bus.
⑧	**AUX CONNECTOR**	A 9-pin D-Subminiature connector for sweep z-axis blanking/penlift (pin 4), and sweep DAC (x-axis) signals (pin 5). It is also for remote control of bright digit and memory sequence up and down operations. See Appendix F for the pinout diagram.

Section 4
Front Panel Operation

INTRODUCTION 4-1.

Section 4 provides instructions for operating the Signal Generator using the front panel controls. The front panel features are described in Section 3.

Each of Sections 4A through 4G describes procedures that are specific to one area of Signal Generator operation. Included with instructions for a particular operation are the equivalent remote (IEEE-488 bus) commands. This is intended to help the remote programmer who needs to refer to the operating instructions while writing a remote program. Refer to Section 5 for complete information about programming the Signal Generator via the IEEE-488 bus.

RECALLING PREVIOUS INSTRUMENT SETTINGS AT POWER-UP 4-2.

Every time you toggle the power off and on, the Signal Generator is reset to the Preset State, as listed in Appendix A. However, the settings that were in effect when the power was turned off are saved in non-volatile memory as instrument state memory location 00. To recall the previous settings, including programmed step sizes, active modes, etc., press [RCL], [0], [0].

For more information about storing and recalling up to 50 different sets of instrument states, refer to Section 4D. For more information about the Preset State and other factory default tables, refer to Appendix A.

ENTERING AND MODIFYING PARAMETERS 4-3.

The six primary parameters of the Signal Generator correspond to the six Function Keys, as follows:

- [FREQ] (RF output frequency)
- [AMPL] (RF output amplitude)
- [AM] (AM depth)
- [FM/ϕM] (FM/ϕM deviation)
- [MOD FREQ] (Modulation frequency)
- [MOD LEV] (Modulation level)

The value of each can be individually set or modified by any of three methods:

- Entering parameters directly
- Editing the bright digit
- Incrementing and decrementing by step

Each of these methods accomplishes the same result, but each method is particularly suited for a specific application. For example, you can establish an initial parameter value by entering it directly, then adjust that parameter with by editing the bright digit or incrementing (or decrementing) it by step.

Entering Parameters Directly 4-4.

To enter a parameter directly, proceed as follows:

1. Select a function.

   Select one of the six functions by pressing a FUNCTION key. The bright digit appears in the corresponding display field. The presence of the bright digit in the display field indicates that the parameter for the selected function is ready to be entered or modified.

2. Enter the numeric data.

   Enter the numeric data using the DATA keys. The numbers appear in the selected display field. The bright digit is off when numeric data is being entered.

3. Enter a unit.

   Press a UNITS key. This gives the numeric data its absolute value and causes the microprocessor to verify that the entered value is within allowable limits and to program the Signal Generator to the new state. The bright digit is redisplayed.

A function remains selected until you press a new FUNCTION key (or send a function remote command). Parameter data for a selected function must be followed by a unit value and must be within the allowable range for the function. If the data is not within the allowable range, the display field flashes, and the REJ ENTRY status annunciator flashes. A rejected entry does not affect the output of the Signal Generator. The output of the Signal Generator remains at its previous setting until a new value is accepted.

You can terminate entry of a function parameter at any time by pressing CLR/LCL or by selecting another function.

Parameter entry commands are provided for remote control of the six functions. Refer to Section 5, "Remote Operation" for more information.

Editing the Bright Digit 4-5.

To adjust the value of a parameter by editing the bright digit, proceed as follows:

1. Select a display field.

   Select one of the six functions using the FUNCTION keys. A bright digit appears in the selected display field.

2. Position the bright digit.

   Use the ◁ or ▷ EDIT keys to position the bright digit on the desired decade of resolution.

3. Adjust the value of the bright digit.

Turn the knob clockwise to increment the bright digit. Turn the knob counterclockwise to decrement the bright digit.

The position of the bright digit within a display field is retained when the bright digit is moved from one display field to another and back to the original field. Note that each function sharing the MODULATION display field (AM Depth, FM/ϕM Deviation, Modulation Frequency and Modulation Level) retains its own bright digit position.

The bright digit is turned off while Manual Sweep is active. Refer to Section 4E for more information about the sweep function.

An edit operation is ignored when the result would cause the value of the edited parameter to exceed its programmable limit.

Bright digit positioning and editing commands are also provided for remote operation for each of the six functions. Refer to Section 5 for more information.

Incrementing and Decrementing by Step 4-6.

You can change the value of a parameter in increments of a programmable step size by pressing the [△] or [▽] STEP keys. The step size for a given function remains in effect until a new step size is selected, even after power is turned off. If you do not initially change the step sizes, the defaults shown in Table 4-1 are in effect.

Table 4-1. Step Size Defaults

PARAMETER	DEFAULT STEP SIZE
Frequency	10 MHz
Amplitude	10 dB
AM Depth	10%
FM/ØM Deviation	1 kHz
Modulation Frequency	1 kHz
Modulation Level	0.1V

To change the magnitude of a step size, proceed as follows:

1. Select the step field.

   Select the field for which you would like to change the step by pressing a FUNCTION key, followed by the [STEP] key to enable the step size entry.

2. Enter data for step size.

   Select the numeric step size using the DATA keys.

3. Select the units.

   Select a UNIT key to give the data its absolute value.

While the [STEP] key is pressed, the display field of the selected parameter shows the step size. The STEP annunciator is lit in the display field affected by the [STEP] key.

The repeat rate of the [△] or [▽] STEP keys may be changed to a faster or slower rate (a medium repeat rate is the default) with a Special Function. Refer to Section 4F for more information about the Special Functions.

A step increment or decrement is ignored when the result of that step would cause the value of the stepped parameter to exceed its programmable limit.

Step entry and step up/down commands are also provided for remote operation for each of the six functions. Refer to Section 5 for more information.

Section 4A
RF Output Frequency

INTRODUCTION 4A-1.

Section 4A describes the procedures for setting the rf output frequency and the associated parameters of rf output frequency.

SETTING RF OUTPUT FREQUENCY 4A-2.

Set the rf output frequency by pressing [FREQ], the necessary DATA keys, and a UNITS key. The rf output frequency is displayed in fixed-point notation in MHz. Pressing [FREQ] key moves the bright digit to the FREQUENCY display field and places the Signal Generator in the rf output frequency entry mode.

RF FREQUENCY

	RANGE	RESOLUTION
6080A	0.01 to 1056	1 Hz
6082A	0.1 to 2112 MHz	1 Hz

SYNTAX:

[FREQ] --Numeric Data-- [MHz|V] [kHz|mV] [Hz|µV]

EXAMPLE: Set rf frequency to 10.7 MHz

FRONT PANEL: [FREQ] [1] [0] [.] [7] [MHz|V]

REMOTE: FREQ 10.7 MHZ

SETTING RF OUTPUT FREQUENCY STEP SIZE 4A-3.

You can change the magnitude of the rf output frequency by programmable step using the [△] and [▽] keys. The default step size is 10 MHz. View the current set step size by holding down [STEP], the step size shows on the display. To change this step size and save your change in non-volatile memory, proceed as follows:

1. Press [FREQ] followed by [STEP] .
2. Enter the data for step size using the DATA keys.
3. Press [MHz|V] or [kHz|mV] to give the data its absolute value. The value you have selected is held momentarily in the FREQUENCY display field.

RF FREQUENCY

	RANGE	RESOLUTION
6080A	0.01 to 1056 MHz	1 Hz
6082A	0.1 to 2112 MHz	1 Hz

SYNTAX:

[FREQ] [STEP] -- Numeric Data-- [MHz|V] [kHz|mV] [Hz|µV]

EXAMPLE: Set rf frequency step size to 103 kHz

FRONT PANEL: [FREQ] [STEP] [1] [0] [3] [kHz|mV]

REMOTE: FREQ_STEP 103 KHZ

USING RF OUTPUT FREQUENCY RELATIVE MODE 4A-4.

The rf output frequency relative mode is useful for establishing a reference frequency and then changing the output relative to that reference. Setting a reference is done by programming the rf output frequency to the desired value, and then enabling the relative mode using a Special Function command from the front panel, or with the FREQ_REL command in remote. This lights the REL annunciator in the FREQUENCY display field, and sets the displayed frequency value to zero. The Signal Generator output does not change during this operation. In relative frequency mode, you can modify parameters as usual: by direct entry, by editing the bright digit, or by increment/decrementing by step.

In relative frequency mode, the rf output frequency is the sum of the reference and the displayed frequency. You can display the rf output frequency by pressing the [FREQ] key. In remote, query the output frequency with the FREQ_ABS? command, and query the reference frequency with the FREQ_BASE? command.

Relative mode may not be enabled or disabled while sweep is active. See Section 4E, "Sweep" for more information.

SYNTAX:

	FRONT PANEL	REMOTE
Turn Relative Frequency Off	SPCL 2 0	FREQ_REL OFF
Turn Relative Frequency On	SPCL 2 1	FREQ_REL ON

ADJUSTING THE PHASE OF THE RF CARRIER 4A-5.

The phase of the rf output carrier can be adjusted relative to another phase coherent signal source using the front panel edit controls. For example, two 6080As or 6082As can be made phase coherent by driving the REF IN on one unit with the 10 MHz OUT from the other unit. The unit receiving the external reference must be set to EXT REF on the rear panel.

Entering SPCL 7 0 1 initiates the carrier phase adjust mode. The message "PHASE" is displayed in the FREQUENCY display field and the initial phase adjustment of zero degrees is displayed in the AMPLITUDE display field. Turn the edit knob to advance/retard the phase in 1 degree or 10 degree increments. The edit ◁ and ▷ keys change the resolution of the bright digit.

The Signal Generator does not measure the phase of the other signal source so it cannot display the absolute phase relationship between the two signals. The display shows the relative phase adjustment applied to the rf output. Pressing the 0 key sets the relative phase adjustment to zero establishing a reference. Press any other key to exit the carrier phase adjust mode.

The relative phase adjustment may also be zeroed by entering SPCL 7 0 2 while outside of the carrier phase adjust mode.

The remote command PHASE adjusts the carrier phase by the specified number of degrees. The relative phase adjustment is updated internally, but is not displayed when the remote commands are received. The command PHASE? queries the relative phase adjustment. The command "PHASE_ZERO" zeros the relative phase adjustment.

The display is momentarily blanked during a phase adjustment.

USING AN EXTERNAL FREQUENCY REFERENCE 4A-6.

The Signal Generator normally derives its output frequency based on a 10-MHz internal reference oscillator. However, if you desire, you can substitute an external source for the internal reference. To use an external reference, set the rear panel REF INT/EXT switch to EXT and connect an external source of 10 MHz ±10 ppm sine wave, 0.2 to 2.0V rms, to the rear panel REF IN connector.

You can also use an external reference of 1, 2, or 5 MHz. One alternate external reference frequency setting is available at a time, through Special Function 761. (Special Function 760 resets the Signal Generator for a 10-MHz external reference.) The default alternate reference frequency is 5 MHz. See the Service Manual for setting internal DIP switches for use with a 1 or 2 MHz external reference.

In remote, use the EXTREF_FREQ command. The selected external reference frequency is in effect whenever the rear panel REF INT/EXT switch is set to EXT.

SYNTAX:

	FRONT PANEL	REMOTE
Select Standard (10MHz) External Reference Frequency	SPCL 7 6 0	EXTREF_FREQ STD
Select Alternate External Reference Frequency	SPCL 7 6 1	EXTREF_FREQ ALT

RF OUTPUT FREQUENCY BANDS 4A-7.

All rf output frequencies are synthesized from a fundamental frequency in the range of 480 to 1056 MHz. This fundamental frequency is divided, heterodyned, or doubled to produce the programmed output frequency. The frequency bands of the Signal Generator are shown in Table 4A-1.

Table 4A-1. Signal Generator Frequency Bands

BAND DESIGNATION	FREQUENCY RANGE (MHz)	DIVIDE RATIO
A (6080A)	.01 to 14.999999	8 (Het)
A (6082A)	0.1 to 14.999999	8 (Het)
B	15 to 31.999999	32
C	32 to 63.999999	16
D	64 to 127.999999	8
E	128 to 255.999999	4
F	256 to 511.999999	2
G (6080A)	512 to 1056	1
G (6082A)	512 to 1055.999999	1
H (6082A)	1056 to 2112	0.5

Section 4B
RF Output Amplitude

INTRODUCTION 4B-1.

Section 4B describes the procedures for programming the rf output amplitude and the associated parameters of rf output amplitude.

SETTING RF OUTPUT AMPLITUDE 4B-2.

The rf output amplitude can be controlled with the FUNCTION-DATA-UNIT entry sequence. The amplitude display is fixed point for dBm and dB units and is floating point for voltage units. The selected unit is retained until a numeric entry is terminated with the alternate unit, the display units are converted, or an alternate dB unit is selected by Special Function. Pressing the [AMPL] function key moves the bright digit to the AMPLITUDE display field and places the Signal Generator in the rf amplitude entry mode.

RF AMPLITUDE

RANGE	RESOLUTION
-147 to +20 dBm 10 nV to 2.24 V	0.1 dBm 3 digits

SYNTAX:

[AMPL] -- Numeric Data -- [dB(m)] [MHz/ V] [kHz/ mV] [Hz/µV]

EXAMPLE: Set Amplitude to -7.5 dBm.

FRONT PANEL: [AMPL] [—] [7] [.] [5] [dB(m)]

REMOTE: AMPL -7.5 DBM

CONVERTING RF OUTPUT AMPLITUDE UNITS 4B-3.

You can convert displayed rf output amplitude quantity from dBm units to voltage units or from voltage units to dBm units by selecting the Amplitude function, then pressing the desired unit key. The output of the Signal Generator does not change during these operations. The display units remain in effect until a numeric entry is terminated with an alternate unit or the display units are converted by reversing the procedure.

AMPLITUDE UNITS CONVERSION:

$$V = 10^{(dBm - 13.0)/20.0}$$

$$dBm = 13.0 + 20.0 \log_{10}(V)$$

SYNTAX:

TO CONVERT	FRONT PANEL	REMOTE
dBm to Volts	AMPL, mV/µV	AMPL_UNITS V
Volts to dBm	AMPL, dB(m)	AMPL_UNITS DBM

SELECTING ALTERNATE DB REFERENCE UNITS 4B-4.

If the rf output amplitude is displayed as a dBm quantity, alternate units of dBmV, dBµV, or dBf may be selected. Selection of an alternate dB reference does not change the output of the Signal Generator. The selected alternate units are retained when changing to or from voltage units, and remain in effect for any Amplitude entry terminated with the dB(m) unit key.

To select an alternate dB reference unit from the front panel, use a Special Function. To select an alternate amplitude unit in remote, use the alternate amplitude unit as the unit terminator for the AMPL command. See Section 5, "Remote Operation" for more information.

ALTERNATE AMPLITUDE UNITS:

dBmV = dBm + 47.0
dBµV=dBm + 107.0
dBf = dBm + 120.0

SYNTAX:

	FRONT PANEL	REMOTE
Select dBm Units	SPCL, 8, 4, 0	AMPL <numeric value> DBM
Select dBmV Units	SPCL, 8, 4, 1	AMPL <numeric value> DBMV
Select dBµV Units	SPCL, 8, 4, 2	AMPL <numeric value> DBUV
Select dBf Units	SPCL, 8, 4, 3	AMPL <numeric value> DBF

USING UNTERMINATED OUTPUT (EMF) MODE 4B-5.

When enabled, unterminated output mode (EMF units) causes amplitude values to be doubled for voltage units, or offset by 6 dB for dBmV or dBμV units. This includes the displayed amplitude, the base amplitude (if the relative amplitude mode is on), the amplitude sweep increment (if in volts), and the amplitude sweep width (if in volts). This also includes all limits to the amplitude values. The unterminated output mode has no effect if the displayed quantity has units of dBm or dBf.

To select the Unterminated Output Display mode from the front panel, use a Special Function. To select the mode in remote, use the AMPL_EMFOUT command.

Enabling this mode has no effect on the Signal Generator output. The EMF units are retained when changing to or from voltage units, and remain in effect for any Amplitude entry based on a voltage unit.

Disabling this mode may change the Signal Generator output since resolution may be lost. For example, an rf output amplitude of 201 mV programmed when in the unterminated output mode will be converted to 100 mV, not 100.5 mV when the mode is disabled.

EMF UNITS CONVERSION:

EMF dBmV = dBmV + 6 dBmV
EMF dBμV = dBμV + 6 dBμV
EMF V = 2*V

SYNTAX:

	FRONT PANEL	REMOTE
Normal Amplitude Display Mode	SPCL 8 5 0	AMPL_EMFOUT OFF
Unterminated Output Display Mode	SPCL 8 5 1	AMPL_EMFOUT ON

SETTING RF OUTPUT AMPLITUDE STEP SIZE 4B-6.

The rf output amplitude step size can be selected for entry by pressing the [AMPL] key, followed by the [STEP] key. As long as the [STEP] key is pressed, the step size is displayed. Upon entering a new step size, the value is held momentarily in the AMPLITUDE display field. Step Increment/Decrement operations are rejected unless the units of the amplitude and amplitude step match.

Note that 0.01 dB resolution is available for amplitude step sizes less than 20.0 dB, even though the rf output amplitude is always displayed with 0.1 dB resolution. In the event that a step size with 0.01 dB resolution is selected, stepping the amplitude up or down may cause the display to become inconsistent with the actual amplitude. Parameter entry of a new rf output amplitude always zeros the 0.01 dB digit; however, bright-digit edit operations retain the 0.01 dB resolution.

RF AMPLITUDE STEP SIZE

RANGE	RESOLUTION
0.00 to 19.99 dB	0.01 dB
20.0 to 167.0 dB	0.1 dB
0 V to 2.24 V	3 digits

SYNTAX:

[AMPL] [STEP] -- Numeric Data -- [dB(m)] [MHz | V] [kHz | mV] [Hz | µV]

EXAMPLE: Set Amplitude Step Size to 6 dB.

FRONT PANEL: [AMPL] [STEP] [6] [dB(m)]

REMOTE: AMPL_STEP 6 DB

USING RF AMPLITUDE RELATIVE MODE 4B-7.

The rf amplitude relative mode lets you establish a reference amplitude then set the output relative to that reference. You set a reference by setting the rf output amplitude to the desired value and then enabling the relative mode using a Special Function command from the front panel, or with the AMPL_REL command in remote. This causes the REL annunciator to light in the AMPLITUDE display field and the displayed value to become zero. The Signal Generator output does not change during this operation. In the relative mode, you can use the usual means of parameter modification: Function Entry, Bright-Digit Edit, or Step Increment/Decrement.

In the relative amplitude mode, the output amplitude is the sum of the reference and the displayed amplitude when the reference and the displayed quantities have the same units. The output amplitude may be displayed by pressing the [AMPL] key. in remote, the output amplitude can be queried with the AMPL_ABS? command and the reference amplitude can be queried with the AMPL_BASE? command.

Note that a reference amplitude having dBm, dBmV, dBμV, or dBf units is converted to a dB (ratio) value, so that the displayed value retains the units of the reference; the output is the displayed value scaled by the reference value. With mixed units (voltage and dB), the output amplitude is the voltage value scaled by the dB value. With voltage units, the output is the sum of the reference and the displayed values. Table 4B-1 illustrates the allowed combinations of reference and displayed amplitude, and shows how the amplitude values are interpreted with the relative amplitude mode enabled.

Relative mode may not be enabled or disabled while sweep is active. See Section 4E, "Sweep" for more information.

SYNTAX:

	FRONT PANEL	REMOTE
Disable Relative Amplitude	SPCL 3 0	AMPL_REL OFF
Enable Relative Amplitude	SPCL 3 1	AMPL_REL ON

EXAMPLE: Compensate for external gain or loss. A +10.0 dB gain amplifier is connected to the output of the Signal Generator. Program the Signal Generator to display the boosted output level using Relative Amplitude.

FRONT PANEL: Press the following keys to program the Signal Generator to -10 dBm. The output of the amplifier is 0.0 dBm

AMPL — 1 0 dB(m)

Press the following keys to select Relative Amplitude. The Signal Generator display now reflects the amplifier output (0.0 dBm).

SPCL 3 1

REMOTE: AMPL 10.0 DBM; AMPL_REL ON

Table 4B-1. Relative Amplitude Unit Combinations

AMPLITUDE WHEN RELATIVE MODE ENABLED	REFERENCE AMPLITUDE UNITS	DISPLAYED AMPLITUDE UNITS	OUTPUT AMPLITUDE (AMPL PRESSED)
dBm	dB	dBm	dBm (displayed) + dB (reference)
dBmV	dB	dBmV	dBmV (displayed) + dB (reference)
dBμV	dB	dBμV	dBμV (displayed) + dB (reference)
dBf	dB	dBf	dBf (displayed) + dB (reference)
dBxx*	dB	voltage	voltage (displayed) x dB (reference)
voltage	voltage	dB	voltage (referenced) x dB (displayed)**
voltage	voltage	voltage	voltage (displayed) + V (reference)**

*Any dB-based units (i.e. dBm, dBμV, dBmV, dBf).
** Units conversion of the displayed amplitude is not allowed when the reference amplitude has Voltage units, since an absolute quantity (Volts) cannot be converted to a ratio (dB).

ENABLING AND DISABLING RF OUTPUT 4B-8.

You can enable and disable the rf output signal by pressing the RF OUTPUT ON/OFF key, or with the RFOUT command in remote. Turning the rf output on resets the Reverse Power Protection (RPP) circuitry if it has been tripped.

Pressing the RF OUTPUT ON/OFF key alternately turns the output off and on. When the rf output is off, the RF OFF annunciator is lit. The amplitude setting when the RF is turned off is restored when the output is turned on again. The displayed amplitude is not changed when the output is turned off.

SYNTAX:

	FRONT PANEL	REMOTE
Turn On RF Output (RF OFF annunciator on)	RF OUTPUT ON/OFF	RFOUT ON
Turn Off RF Output (RF OFF annunciator off)	RF OUTPUT ON/OFF	RFOUT OFF

RF OUTPUT AMPLITUDE BANDS 4B-9.

Amplitude settings for the Signal Generator are achieved by cascading the rf output through a series of attenuators for coarse control and through a DAC for vernier control. The attenuator series consists of a single 6-dB section, a single 12-dB section, and five 24-dB sections. When Amplitude Modulation (AM) is enabled, the amplitude band switch points are shifted down by 3 dB (6080A) or 6 dB (6082A). Table 4B-2 depicts the amplitude band divisions of the Signal Generator in dBm units.

Table 4B-2. RF Output Amplitude Bands

AMPLITUDE RANGE IN dBm					
AM OFF		AM ON (6080A)		AM ON (6082A)	
+7.0	+20.0	+4.0	+20.0	+1.0	+20.0
+1.0	+6.9	–2.0	+3.9	–5.0	+0.9
–5.0	+0.9	–8.0	–2.1	–11.0	–5.1
–11.0	–5.1	–14.0	–8.1	–17.0	–11.1
–17.0	–11.1	–20.0	–14.1	–23.1	–17.1
–23.1	–17.1	–26.1	–20.1	–29.1	–23.2
–29.1	–23.2	–32.1	–26.2	–35.1	–29.2
–35.1	–29.2	–38.1	–32.2	–41.1	–35.2
–41.1	–35.2	–44.1	–38.2	–47.1	–41.2
–47.1	–41.2	–50.1	–44.2	–53.2	–47.2
–53.2	–47.2	–56.2	–50.2	–59.2	–53.3
–59.2	–53.3	–62.2	–56.3	–65.2	–59.3
–65.2	–59.3	–67.2	–62.3	–71.2	–65.3
–71.2	–65.3	–73.2	–68.3	–77.2	–71.3
–77.2	–71.3	–80.3	–74.3	–83.3	–77.3
–83.3	–77.3	–86.3	–80.4	–89.3	–83.4

Table 4B-2. RF Output Amplitude Bands (cont)

AMPLITUDE RANGE IN dBm					
AM OFF		AM ON (6080A)		AM ON (6082A)	
–89.3	–83.4	–92.3	–86.4	–95.3	–89.4
–95.3	–89.4	–98.3	–92.4	–101.3	–95.4
–101.3	–95.4	–104.4	–98.4	–107.4	–101.4
–107.4	–101.4	–110.4	–104.5	–113.4	–107.5
–113.4	–107.5	–116.4	–110.5	–119.4	–113.5
–119.4	–113.5	–122.4	–116.5	–125.4	–119.5
–125.4	–119.5	–128.4	–122.5	–131.5	–125.5
–147.0	–125.5	–147.0	–128.5	–147.4	–131.6

USING RF OUTPUT AMPLITUDE FIXED-RANGE MODE 4B-10.

When enabled, Amplitude Fixed-Range mode fixes the setting of the attenuators at the given output level. This allows monotonic and nontransient level control over a limited range around those levels where the attenuators are normally reranged.

Fixed-range mode is enabled using a Special Function command from the front panel, or with the AMPL_RANGE command in remote. The SPCL annunciator is lit when fixed-range mode is enabled. Fixed-range level control remains in effect only during Bright-Digit Edit of the AMPLITUDE display field. Other methods of changing the output cause the attenuators to rerange if necessary. Changing the rf output frequency, initiating an rf amplitude sweep, or enabling/disabling AM will also cause the attenuators to rerange.

The level vernier in fixed-range mode has a specified accuracy range of 12 dB around the point at which fixed-range mode is enabled. If an attempt is made to edit the amplitude value beyond the range of the vernier, the STATUS annunciator flashes, and the output level is not guaranteed.

SYNTAX:

	FRONT PANEL	REMOTE
Disable Fixed-Range	SPCL 5 0	AMPL_RANGE NORMAL
Enable Fixed-Range	SPCL 5 1	AMPL_RANGE FIXED

EXAMPLE: Set the Signal Generator for monotonic and nontransient amplitude control (Bright-Digit Edit only) over the range of the vernier level control below 0.25V.

FRONT PANEL: AMPL . 2 5 MHz|V SPCL 5 1

REMOTE: AMPL 0.25 V ; AMPL_RANGE FIXED

USING ALTERNATE OUTPUT COMPENSATION MODES 4B-11.

Alternate output compensation modes are available on the Signal Generator. Normally, a factory-generated set of data which characterizes the output circuitry is applied, and a factory-generated set of data which characterizes the attenuators is applied. It is possible to configure the Signal Generator to apply the output circuitry compensation data only (no attenuator compensation) to the output, or to apply no compensation data to the output. Selecting a compensation mode is done using a Special Function command from the front panel, or with the AMPL_COMP command in remote. The SPCL annunciator is lit when an alternate compensation mode is selected.

SYNTAX:

	FRONT PANEL	REMOTE
Apply All Compensation Data	SPCL 9 2 0	AMPL_COMP ALL
Apply No Compensation Data*	SPCL 9 2 1	AMPL_COMP NONE
Apply Output Compensation Only	SPCL 9 2 2	AMPL_COMP OUTPUT

* NOTE: Also disables Level Calibration

SELECTING ALTERNATE OUTPUT COMPENSATION DATA 4B-12.

The Signal Generator has provision for user-definable output (output circuitry) compensation data. It is possible to characterize the Signal Generator when the rf output is connected through a lengthy or lossy path and store this data. The method for generating this data this is described in the Signal Generator Service Manual. Once an alternate set has been loaded, the alternate compensation data can be selected for use using a Special Function command from the front panel, or with the AMPL_CMPDAT command in remote. The SPCL annunciator is lit when alternate compensation data are selected.

SYNTAX:

	FRONT PANEL	REMOTE
Apply Standard Output Compensation Data	SPCL 9 3 0	AMPL_CMPDAT STD
Apply Alternate Output* Compensation Data	SPCL 9 3 1	AMPL_CMPDAT ALT

* NOTE: This compensation data is only applied to the Output Circuitry.

Section 4C
Modulation

INTRODUCTION 4C-1.

The Signal Generator offers four modulation capabilities:

- Amplitude modulation (AM)
- Frequency modulation (FM)
- Phase modulation (ϕM)
- Pulse modulation (⎍)

The MODULATION ON/OFF keys enable and disable one or more types of modulation from internal and external sources. Each modulation key is a toggle on/off type. Annunciators in the MODULATION display field indicate the enabled modulation types.

Various combinations of AM, FM/ϕM, and pulse modulation may be enabled in either internal or external (or both) modes. Some restrictions exist for certain combinations:

- FM and ϕM are always mutually exclusive
- External ac and dc modes of each modulation form are mutually exclusive.

It is easier to understand by considering AM, FM/ϕM, and pulse modulation as three separate groups, where FM and ϕM are mutually exclusive members of a single group. While interactions and exclusions exist within each group, there are no interactions between groups. In other words, no combination of AM on/off modes ever interacts with FM/ϕM on/off modes, or pulse modulation on/off modes.

The MODULATION display field is shared by amplitude modulation depth, frequency/phase modulation deviation, modulation frequency, and modulation level. Since there is only one modulation display, the displayed modulation parameter is determined by the last modulation FUNCTION key pressed.

INTERNAL MODULATION OSCILLATOR 4C-2.

An internal modulation oscillator digitally synthesizes one of three waveforms (sine, square, triangular) at a specified modulation frequency. The internal modulation oscillator uses DDS (Direct Digital Synthesis) to provide excellent signal purity. It can also be configured as a pulse generator where the pulse width and repetition rate are programmable. The synthesized modulation waveform is available at the front panel connector labeled MOD OUTPUT.

Setting Modulation Frequency and Step Size 4C-3.

The modulation frequency (Mod Frequency) is displayed in the Signal Generator front panel MODULATION display field with three digits of resolution. The Mod Frequency is displayed with kHz or Hz units, with the MOD FREQ annunciator on.

Mod Frequency and the Mod Frequency Step Size are controlled using the FUNCTION-DATA-UNIT entry sequence. Pressing the [MOD FREQ] function key causes the MODULATION display field to display the Mod Frequency, moves the bright digit to the MODULATION display field and places the Signal Generator in the Mod Frequency entry mode. Entry or modification of the Mod Frequency does not change the Signal Generator's rf output unless internal modulation is enabled. The Mod Frequency step size is selected for entry by pressing the [STEP] key after selecting the Mod Frequency function.

As a shortcut method, use the [400/1000] key to toggle the Mod Frequency between 400 and 1000 Hz. The MODULATION display field is updated to reflect 400 Hz or 1.00 kHz as the values are selected. This key is inactive when the front panel bright digit is turned off.

MODULATION FREQUENCY

RANGE	RESOLUTION
0.1 Hz to 200 kHz	3 digits

SYNTAX:

Modulation Frequency

[MOD FREQ] -- numeric data -- [MHz|V] [kHz|mV] [Hz|µV]

Modulation Frequency Step Size

[MOD FREQ] [STEP] -- numeric data -- [MHz|V] [kHz|mV] [Hz|µV]

EXAMPLE 1: Set Modulation Frequency to 19 kHz

FRONT PANEL: [MOD FREQ] [1] [9] [kHz|mV]

REMOTE: MODF 19 KHZ

EXAMPLE 2: Set Modulation Frequency Step Size to 1 kHz

FRONT PANEL: [MOD FREQ] [STEP] [1] [kHz|mV]

REMOTE: MODF_STEP 1 KHZ

Setting Modulation Level and Step Size 4C-4.

Modulation level refers to the peak level signal present at the front panel connector (labeled MOD OUTPUT), into a 600Ω load. The modulation level (Mod Level) is displayed in the Signal Generator front panel MODULATION display field with three digits of resolution. The Mod Level is displayed with V units, with the MOD LEVEL annunciator on.

The Mod Level and Mod Level step size are controlled using the FUNCTION-DATA-UNIT entry sequence. Pressing the [MOD LEV] key causes the MODULATION display field to display the current Mod Level, moves the bright digit to the MODULATION display field, and places the Signal Generator in the Mod Level entry mode. The Mod Level setting has no effect on the Signal Generator rf output. The Mod Level step size is selected for entry by pressing the [STEP] key after selecting the Mod Level function.

MODULATION LEVEL

RANGE	RESOLUTION
0.0 to 4.00 V	3 digits

MODULATION LEVEL STEP SIZE

RANGE	RESOLUTION
0.0 to 4.00 V	3 digits

SYNTAX:

Modulation Level

[MOD LEV] -- numeric data -- [MHz|V] [kHz|mV] [Hz|µV]

Modulation Level Step Size

[MOD LEV] [STEP] -- numeric data-- [MHz|V] [kHz|mV] [Hz|µV]

EXAMPLE 1: Set Modulation Level to 1.41 v

FRONT PANEL: [MOD LEV] [1] [.] [4] [1] [MHz|V]

REMOTE: MODL 1.41 V

EXAMPLE 2: Set Modulation Level Step Size to 1 mV

FRONT PANEL: [MOD LEV] [STEP] [1] [kHz|mV]

REMOTE: MODL_STEP 1 MV

Enabling and Disabling Modulation Output 4C-5.

Output of the internal modulation oscillator signal through the MOD OUTPUT connector on the front panel may be enabled and disabled. Note that the internal modulation signal is normally output through this connector, even though all internal modulation is off. To disable the modulation output, use a Special Function from the front panel, or the MODOUT command in remote. The SPCL annunciator is lit when the modulation output is disabled.

SYNTAX:

	FRONT PANEL	REMOTE
Turn Off Modulation Output	SPCL 4 1	MODOUT OFF
Turn On Modulation Output	SPCL 4 0	MODOUT ON

Selecting the Internal Modulation Waveform 4C-6.

The Signal Generator internal modulation oscillator is capable of producing a variety of output waveforms. These waveforms are: sine wave, triangle wave, and square wave. The oscillator may also be configured as a variable width pulse generator. Only one of the waveforms, or the internal pulse generator mode can be enabled at any given time.

The selected waveform may be applied to the internal AM, internal FM, or internal pulse circuitry. Each modulation path (AM, FM, pulse) is controlled independently of the others.

This selection scheme allows any waveform to be applied to internal AM, internal FM, or internal pulse. In addition, multiple modulation paths (e.g., internal AM and internal FM) may be simultaneously enabled to use the selected waveform, although the resulting output may be of little use.

The SPCL annunciator is lit when an alternate modulation waveform is selected. The following Front Panel key sequences and Remote commands select the waveform of the modulation oscillator:

SYNTAX:

WAVEFORM	FRONT PANEL	REMOTE
Sine	SPCL 7 5 0	MOD_WAVE SINE
Triangle	SPCL 7 5 1	MOD_WAVE TRIANGLE
Square	SPCL 7 5 2	MOD_WAVE SQUARE

Using the Extended Resolution Mode for Modulation Frequency 4C-7.

An extended resolution mode is available for entry of Mod Frequency. This mode is enabled with a Special Function command and allows the Mod Frequency to be input from the front panel with 0.1Hz resolution over its entire range. This resolution is always available in remote using the "MODF" command.

Entering [SPCL] [4] [2] displays the current modulation frequency in the FREQUENCY display field with 0.1 Hz resolution followed by a question mark prompt which indicates that a new modulation frequency can be entered. If a new modulation frequency is entered in response to the prompt, it is rounded to 0.1 Hz resolution and the modulation oscillator circuitry is programmed accordingly. The new modulation frequency is displayed in the MODULATION display field. If it has more than three significant digits, it is rounded to three digits before it is displayed.

Mod Frequency entries are stored in two formats: with the displayed 3-digit resolution and with extended 0.1 Hz resolution. Every Mod Frequency or extended resolution Mod Frequency entry is stored in both formats. However, step, edit, store and recall operations operate on the displayed value only. Extended resolution Mod Frequency entries are temporary entries, in that any edit or step increment/decrement operations force the value back into normal resolution. Only Special Function 42 will display an extended entry with full resolution, and only if no intervening commands have truncated it.

SYNTAX:

[SPCL] [4] [2] -- Numeric Data-- [MHz/V] [kHz/mV] [Hz/µV]

AMPLITUDE MODULATION (AM) 4C-8.

Amplitude modulation depth is displayed in the Signal Generator modulation display field with 0.1% of resolution. The AM depth is displayed with "%" units.

Note that internal AM can be combined with external ac-coupled AM (ACAM) or external dc-coupled AM (DCAM). However, external ACAM and external DCAM are mutually exclusive. Enabling external ACAM while external DCAM is enabled turns off external DCAM, and vice versa.

Setting AM Depth and AM Depth Step Size 4C-9.

The AM depth and AM depth step size are controlled using the FUNCTION-DATA-UNIT entry sequence. Pressing the [AM] function key causes the MODULATION display field to display the AM depth, moves the bright digit to the MODULATION display field and places the Signal Generator in the AM depth entry mode. Entry or modification of the AM depth value does not change the Signal Generator output unless AM is enabled. The AM depth step size is selected for entry by pressing the [STEP] key after selecting the AM function.

AM DEPTH

RANGE	RESOLUTION
0 to 99.9%	0.1%

AM DEPTH STEP SIZE

RANGE	RESOLUTION
0 to 99.9%	0.1%

SYNTAX:

Set AM Depth

[AM] -- numeric data -- [%/rad]

Select AM Depth Step Size

[AM] [STEP] -- numeric data -- [%/rad]

EXAMPLE 1: Set AM depth to 23.5%

FRONT PANEL: [AM] [2] [3] [.] [5] [%/rad]

REMOTE: AM 23.5 PCT

EXAMPLE 2: Set AM depth step size to 1.0%

FRONT PANEL: [AM] [STEP] [1] [%/rad]

REMOTE: AM_STEP 1.0 PCT

Activating Internal AM 4C-10.

Internal AM is enabled by pressing the [INT AM] key from the front panel, or using the INT_AM ON command in remote. The INT AM annunciator is lit when Internal AM is enabled. With Internal AM enabled, the internal modulation oscillator modulates the rf signal to the specified AM Depth at the modulation frequency rate. This rate may be viewed by pressing [MOD FREQ] . Pressing the [INT AM] key again disables internal AM, as does the INT_AM OFF command in remote.

Activating External AM (AC Coupled) 4C-11.

External ac-coupled AM (ACAM) is enabled by pressing the [EXT AC AM] key from the front panel, or with the EXTAC_AM ON command in remote. The EXT AM annunciator is lit when External AM is enabled. When external AM is enabled, the modulating signal is applied through the front panel external AM input connector. Pressing the [EXT AC AM] key again disables External AM, as does the EXTAC_AM OFF command in remote.

External AM uses a 1V pk input signal. Two annunciators on the front panel give indications of when the external ACAM modulation signal is outside the range of 1V ±2%. These annunciators are lit only when external ACAM is enabled and are not active when external DCAM is enabled. If the signal is greater than 1.02V, the AM HI annunciator is lit. If the signal is less than 0.98V, the AM LO annunciator is lit.

Activating External AM (DC Coupled) 4C-12.

External dc-coupled AM (DCAM) is enabled by pressing the [EXT DC AM] key from the front panel, or using with the EXTDC_AM ON command in remote. The EXT DC AM annunciator is lit when External AM is enabled. When external AM is enabled, the modulating signal is applied through the front panel external AM input connector. External AM is normalized for a 1V pk input signal. Pressing the [EXT DC AM] key again disables External DC AM, as does the EXTDC_AM OFF command in remote.

FREQUENCY AND PHASE MODULATION (FM/ϕM) 4C-13.

Frequency modulation (FM) deviation and phase modulation (ϕM) deviation are displayed in the Signal Generator front panel MODULATION display field with three digits of resolution. FM is displayed with MHz DEV, kHz DEV, or Hz DEV units, and ϕM is displayed with rad units.

ϕM entries and modifications are processed internally as FM after the ϕM deviation is converted to an equivalent FM deviation. The modulation circuitry is configured to maintain this relationship over the range of allowed modulation frequencies and deviations. Because of this direct relationship between FM and ϕM, this section focuses on FM programming, with references to ϕM where appropriate.

NOTE

FM and ϕM are always mutually exclusive. For FM, external ACFM and external DCFM are mutually exclusive. For ϕM, external ACϕM and external DCϕM are mutually exclusive. Enabling external ACFM while external DCFM is enabled, turns off external DCFM, and vice versa. The same holds true for ϕM.

Setting FM/ϕM Deviation and FM/ϕM Step Size 4C-14.

The FM/ϕM deviation and FM/ϕM deviation step size are controlled using the FUNCTION-DATA-UNIT entry sequence. Pressing the FM/ϕM deviation function key [FM|ϕM] causes the MODULATION display field to display the current FM/ϕM deviation, moves the bright digit to the MODULATION display field, and places the Signal Generator in the FM/ϕM deviation entry mode. Entry or modification of the FM/ϕM deviation value does not change the Signal Generator output unless FM/ϕM is enabled.

The FM/ϕM deviation step size is selected for entry by pressing the [STEP] key after selecting the FM/ϕM function. Although the FM/ϕM deviation and FM/ϕM deviation step size may have different units, Step Increment and Decrement operations are rejected unless the units are consistent.

FM/ϕM DEVIATION

		RANGE	RESOLUTION
6080A	FM	0 to 4.00 MHz	3 digits
	ϕM	0 to 400 rad	3 digits

		RANGE	RESOLUTION
6082A	FM	0 to 4.00 MHz	3 digits
	ϕM	0 to 4.00 rad	3 digits

FM/ϕM DEVIATION STEP SIZE

		RANGE	RESOLUTION
6080A	FM	0 to 8.00 MHz	3 digits
	ϕM	0 to 8.00 rad	3 digits

		RANGE	RESOLUTION
6082A	FM	0 to 4.0 MHz	3 digits
	ϕM	0 to 400 rad	3 digits

SYNTAX:

Set FM Deviation

FM|ϕM -- numeric data -- MHz|V / kHz|mV / Hz|µV

Set ϕM Deviation

FM|ϕM -- numeric data -- %|rad

Select FM deviation step size

FM|ϕM STEP -- numeric data -- MHz|V / kHz|mV / Hz|µV

Select ϕM deviation step size

FM|ϕM STEP -- numeric data -- %|rad

EXAMPLE 1: Set FM deviation to 50 kHz

FRONT PANEL: FM|ϕM 5 0 kHz|mV

REMOTE: FM 50 KHZ

EXAMPLE 2: Set FM deviation step size to 500 Hz

FRONT PANEL: FM|ϕM STEP 5 0 0 Hz|µV

REMOTE: FM_STEP 500 HZ

The maximum FM/ϕM deviation allowed when FM or ϕM is enabled depends on the rf output frequency. Deviations up to 4 MHz/400 radians (6080A) or 8 MHz/800 radians (6082A) may be entered regardless of the output frequency; however, the STATUS annunciator is flashed if FM/ϕM modulation is enabled and the limits specified in Table 4C-1 are exceeded.

Table 4C–1. FM/ØM Deviation Limits (FM/ØM Enabled)

FREQUENCY BAND (MHz)	MAXIMUM FM DEVIATION	MAXIMUM ØM DEVIATION
.01 to 15 (6080A)	500 kHz	50.0 radians
.1 to 15 (6082A)	500 kHz	50.0 radians
15 to 32	125 kHz	12.5 radians
32 to 64	250 kHz	25.0 radians
64 to 128	500 kHz	50.0 radians
128 to 256	1.0 MHz	100 radians
256 to 512	2.0 MHz	200 radians
512 to 1056	4.0 MHz	400 radians
1056 to 2112 (6082A)	8.0 MHz	800 radians

Converting FM/ϕM Units 4C-15.

When converting from FM deviation to ϕM deviation and vice versa, the output of the Signal Generator does not change. However, the programmed modulation frequency must be taken into account, specifically:

FM deviation (Hz) = ϕM deviation (rad) * Modulation Frequency (Hz)

ϕM deviation (rad) = FM deviation (Hz)/ Modulation Frequency (Hz)

The Mod Frequency used in these equations is always that of the internal modulation oscillator. Note that certain combinations of modulation frequency and the FM deviation or ϕM deviation may not be converted into the alternate units if the resulting deviation is outside the range allowed for those units.

Since the frequency of an external modulation source cannot be determined, FM/ϕM units conversion is rejected if external FM or ϕM is enabled.

SYNTAX:

TO CONVERT	FRONT PANEL	REMOTE
FM to ϕM	FM|ϕM, rad	FM_UNITS RAD
ϕM to FM	FM|ϕM, MHz|V / kHz|mV / Hz|μV	FM_UNITS HZ

Activating Internal FM/ϕM 4C-16.

Internal FM/ϕM is enabled by pressing the [INT FM/ϕM] key from the front panel or with the INT_FM ON command in remote. The unit specified for the FM deviation determines if the INT FM or INT ϕM annunciator is lit when Internal FM/ϕM is enabled. With Internal FM/ϕM enabled, the internal modulation oscillator modulates the rf output to the specified FM deviation or ϕM phase angle at the modulation frequency rate. This rate may be viewed by pressing [MOD FREQ] . Pressing the [INT FM/ϕM] key again disables Internal FM/ϕM, as does the INT_FM OFF command in remote.

Activating External FM/ϕM (AC Coupled) 4C-17.

External AC-coupled FM/ϕM (ACFM) is enabled by pressing the [EXT AC FM/ϕM] key from the front panel, or with the EXTAC_FM ON command in remote. The EXT FM annunciator is lit when External FM is enabled, and the EXT ϕM annunciator is lit when External ϕM is enabled. When either is enabled, the modulating signal is applied through the front panel external FM/ϕM input connector. Pressing the [EXT AC FM/ϕM] key again disables External FM/ϕM, as does the EXTAC_FM OFF command in remote.

External FM/ϕM uses a 1V pk input signal. Two annunciators on the front panel give indications of when the external ACFM or ACϕM modulation signal is outside the range of 2% of 1V. These annunciators are only lit when external ACFM or ACϕM is enabled and are not active when external DCFM or DCϕM is enabled. If the signal is more than 1.02V, the FM HI annunciator is lit. If the signal is less than 0.98V, the FM LO annunciator is lit.

Activating External FM (DC Coupled) 4C-18.

External DCFM is enabled by pressing the [EXT DC FM/ϕM] key from the front panel, or with the EXTDC_FM ON command in remote. The EXT DC FM annunciator is lit when External FM is enabled, and the EXT DC ϕM annunciator is lit when External DC ϕM is enabled. When either is enabled the modulating signal is applied through the front panel external FM/ϕM input connector. External FM/ϕM is normalized for a 1V pk input signal. Pressing the [EXT AC FM/ϕM] key again disables External FM/ϕM, as does using the EXTDC_FM OFF command in remote.

The external DCFM mode allows the rf signal to be frequency modulated by dc or by slowly varying ac rates by an input signal connected to the front panel FM/ϕM MODULATION INPUT connector. Enabling DCFM selects the dc-coupled path from the external FM/ϕM connector and forces the FM circuitry to search for a correction voltage that maintains the rf frequency when the FM loop is unlocked. The FM loop is then configured to the unlocked state.

This search for the FM loop correction voltage is called a DCFM "cal cycle". The time required to perform a DCFM cal cycle is determined by the selected FM band (see Section 4C-13). In most cases, the DCFM cal cycle completes in 0.5 seconds. However, if FM deviation in excess of 250 kHz is selected, the DCFM cal cycle can take up to 5 seconds. Once DCFM has been enabled, the message "PAUSE" appears in the FREQUENCY display field. When the hardware has settled, the display returns to its normal state.

While DCFM is enabled, the rf output frequency will drift with time. To remove the offset caused by this drift, a DCFM cal cycle should be performed as necessary. To force a DCFM cal cycle to occur, ACFM should be enabled (by pressing the EXT AC FM/φM key), followed by re-enabling DCFM.

External DC ϕM is identical to external AC ϕM except that the external FM/ϕM modulation input is dc coupled. Pressing the EXT DC FM/φM key while the FM/ϕM display shows ϕM in radians units, enables the dc-coupled path from the external FM/ϕM input connector, and enables the FM/ϕM circuitry programmed in the phase modulation mode. The external DCϕM mode is entirely different from external DCFM, as the FM oscillator loop remains locked.

FM Bands 4C-19.

The interdependence between rf output frequency bands and FM bands is summarized in Tables 4C-2 and 4C-3. Table 4C-2 shows the FM band limits for normal FM mode. Table 4C-3 shows these limits when Low-Distortion FM is enabled. Each table is a two-dimensional matrix: the column entries represent rf output frequency bands, and the row entries represent each FM band. Each box lists the FM deviations that correspond to the upper and lower limits for that intersection of FM band and rf output frequency band.

Table 4C-2. FM Band Limits

	FREQUENCY BAND (MHz)						
FM RANGE	1056-2112 (6082A)	512-1056	256-512	128-256	64 -128 Het	32 - 64	15 - 32
6	8.00 MHz 2.01 MHz	4.00 MHz 1.01 MHz	2.00 MHz 501 kHz	1.00 MHz 251 kHz	500 kHz 126 kHz	250 kHz 62.6 kHz	125 kHz 31.3 kHz
5	2.00 MHz 501 kHz	1.00 MHz 251 kHz	500 kHz 126 kHz	250 kHz 62.6 kHz	125 kHz 31.3 kHz	62.5 kHz 15.7 kHz	31.2 kHz 7.82 kHz
4	500 kHz 126 kHz	250 kHz 62.6 kHz	125 kHz 31.3 kHz	62.5 kHz 15.7 kHz	31.2 kHz 7.82 kHz	15.6 kHz 3.91 kHz	7.81 kHz 1.96 kHz
3	125 kHz 31.3 kHz	62.5 kHz 15.7 kHz	31.2 kHz 7.82 kHz	15.6 kHz 3.91 kHz	7.81 kHz 1.96 kHz	3.90 kHz 977 Hz	1.95 kHz 489 Hz
2	31.2 kHz 7.82 kHz	15.6 kHz 3.91 kHz	7.81 kHz 1.96 kHz	3.90 kHz 977 Hz	1.95 kHz 489 Hz	976 Hz 245 Hz	488 Hz 123 Hz
1	7.81 kHz 0 Hz	3.90 kHz 0 Hz	1.95 kHz 0 Hz	976 Hz 0 Hz	488 Hz 0 Hz	244 Hz 0 Hz	122 Hz 0 Hz
0	CW MODE						

Table 4C-3. FM Band Limits - Low Distortion Mode

FM RANGE	FREQUENCY BAND (MHz)						
	1056-2112 (6082A)	512-1056	256-512	128-256	64 -128 Het	32 - 64	15 - 32
6	8.00 MHz 2.01 MHz	4.00 MHz 1.01 MHz	2.00 MHz 501 kHz	1.00 MHz 251 kHz	500 kHz 126 kHz	250 kHz 62.6 kHz	125 kHz 31.3 kHz
5	2.00 MHz 501 kHz	1.00 MHz 251 kHz	500 kHz 126 kHz	250 kHz 62.6 kHz	125 kHz 31.3 kHz	62.5 kHz 15.7 kHz	31.2 kHz 7.82 kHz
4	500 kHz 56.1 kHz	250 kHz 28.1 kHz	125 kHz 14.1 kHz	62.5 kHz 7.01 kHz	31.2 kHz 3.51 kHz	15.6 kHz 1.76 kHz	7.81 kHz 876 Hz
3	56.0 kHz 31.3 kHz	28.0 kHz 15.7 kHz	14.0 kHz 7.81 kHz	7.00 kHz 3.91 kHz	3.50 kHz 1.96 kHz	1.75 kHz 977 Hz	875 Hz 489 Hz
2	31.2 kHz 4.01 kHz	15.6 kHz 2.01 kHz	7.80 kHz 1.01 kHz	3.90 kHz 501 Hz	1.95 kHz 251 Hz	976 Hz 126 Hz	488 Hz 63 Hz
1	4.00 kHz 0 Hz	2.00 kHz 0 Hz	1.00 kHz 0 Hz	500 Hz 0 Hz	250 Hz 0 Hz	125 Hz 0 Hz	62 Hz 0 Hz
0	CW MODE						

Using Low Distortion and Fixed-Range FM Modes 4C-20.

Two modes are available to modify or limit the ranging of the FM circuitry. These modes offer improved performance of the FM circuitry for certain applications. These modes are enabled using a Special Function command from the front panel, or with the FM_RANGE command in remote. Entering either of these modes lights the SPCL annunciator below the FREQUENCY display field.

In the normal operation mode, the optimal FM band is determined for the specified combination of rf output frequency and FM deviation.

In FM Low Distortion mode, the total harmonic distortion is diminished, with a corresponding increase in phase noise. This mode provides the optimum phase noise-to-distortion performance at 3.5-kHz FM deviation at Mod Frequencies of 0.3 to 3 kHz.

In FM Fixed-Range mode, total harmonic distortion is improved over a wide range of FM deviation, with the lowest distortion near the lower end of each FM band. In this mode, it is possible to edit above or below the normal FM band limits since the normal FM autorange function is inhibited. The Fixed-Range mode locks to the FM band so that all subsequent adjustments made to the FM deviation and the rf output frequency with the edit knob are processed without the auto-range. If an attempt is made to edit either of these values beyond the range limit, the STATUS annunciator flashes, and the value is constrained to the limit.

When FM Fixed-Range mode is enabled, FM deviation or step entries that map into FM ranges other than the current range will cause the FM circuitry to rerange. Fixed-Range mode remains in effect with the new FM range locked in. In addition, a change in the rf output frequency can also force a FM rerange.

SYNTAX:

	FRONT PANEL	REMOTE
Normal FM Ranging Mode	SPCL 7 3 0	FM_RANGE NORMAL
Low Distortion FM Mode	SPCL 7 3 1	FM_RANGE LOWDISTORT
Fixed-Range FM Mode	SPCL 7 3 2	FM_RANGE FIXED

Using Low Rate FM Mode 4C-21.

Certain applications require FM at low modulation rates but cannot tolerate the shortcomings associated with operating in the DCFM mode when the FM loop is unlocked. When Low-Rate FM is enabled, lower modulation rates may be applied.

Low Rate FM mode is enabled with a Special Function command from the front panel, or with the LORATEFM command in remote. Although the mode is enabled, the FM circuitry is not set to the low-rate configuration unless internal FM or external FM is also enabled. Enabling this function does not affect the circuitry if the Signal Generator is programmed for phase modulation.

When the low-rate FM mode is enabled, the SPCL annunciator in the FREQUENCY display field is lit. The LO RATE annunciator in the MODULATION display field is lit when internal or external FM is enabled.

SYNTAX:

	FRONT PANEL	REMOTE
Turn Low Rate FM Off	SPCL 7 1 0	LORATEFM OFF
Turn Low Rate FM On	SPCL 7 1 1	LORATEFM ON

Using High Rate ϕM Mode 4C-22.

The high-rate ϕM mode trades higher modulation rates (up to 100 kHz) for less phase modulation deviation. Up to 40 radians of phase deviation are allowed in this mode.

High Rate ϕM mode is enabled with a Special Function command from the front panel, or with the HIRATEPM command in remote. When the high-rate ϕM mode is enabled, the SPCL annunciator in the FREQUENCY display field is lit.

SYNTAX:

	FRONT PANEL	REMOTE
Disable High Rate ϕM	SPCL 7 2 0	HIRATEPM OFF
Enable High Rate ϕM	SPCL 7 2 1	HIRATEPM ON

PULSE MODULATION 4C-23.

External and internal pulse modulation are supported in the Signal Generator. Both internal and external pulse modulation may be enabled simultaneously. External pulse modulation input is always dc coupled.

Activating External Pulse Modulation 4C-24.

External Pulse is enabled by pressing the [EXT ⎍] key from the front panel, or with the EXT_PULSE ON command in remote. The EXT ⎍ annunciator is lit when External Pulse is enabled. Pressing the [EXT ⎍] key again disables External Pulse Mode, as does the EXT_PULSE OFF command in remote.

External pulse modulation input is always dc coupled, and can be driven by a TTL-compatible signal. External pulse modulation is triggered at a 1V threshold crossing; any modulating signal applied to the EXT ⎍ front panel connector causes full scale output when the input signal exceeds the threshold and full attenuation when the input signal is below the threshold.

Activating Internal Pulse Modulation 4C-25.

Internal Pulse is enabled with a Special Function command from the front panel, or with the INT_PULSE command in remote. The INT ⎍ annunciator is lit when Internal Pulse is enabled.

Internal Pulse mode is usable with any internal modulation oscillator waveform. A special mode of pulse modulation, with variable pulse width, is described in paragraph 4C-16 ("Internal Pulse Generator Mode").

SYNTAX:

	FRONT PANEL	REMOTE
Turn Off Internal Pulse Modulation	[SPCL] [7] [4] [0]	INT_PULSE OFF
Turn On Internal Pulse Modulation	[SPCL] [7] [4] [1]	INT_PULSE ON

Using the Mod Oscillator as a Pulse Generator 4C-26.

The internal modulation oscillator can be configured as a variable width pulse generator. When configured in this mode, the internal mod oscillator generates a free running pulse train. Triggering of this pulse train is not possible.

Selecting the pulse generator mode in conjunction with the internal pulse modulation path provides internal pulse modulation with variable duty cycle. Pulse periods in the range of 100 ms to 5 μs are available by programming the Mod Frequency in the range from 10 Hz to 200 kHz. If a pulse period less than the pulse width is specified, the STATUS annunciator is flashed, and a pulse width that is 0.1 μs less than the pulse period is substituted.

The pulse period is given priority over the pulse width. However, if a Mod Frequency is entered that would result in a pulse period less than the stored pulse width, the pulse width will be programmed to 0.1 μs less than the pulse period.

Modulation frequencies less than 10 Hz (pulse periods greater than 100 ms) can be entered; however, the STATUS annunciator is flashed and the pulse period is programmed to 100 ms.

The internal pulse generator mode is enabled with a Special Function command from the front panel or with the MOD_WAVE command in remote.

Setting Pulse Width 4C-27.

When the modulation oscillator is configured as a variable width pulse generator, any pulse width in the valid range may be entered using a Special Function command from the front panel or the PULSE_WIDTH command from Remote.

The pulse width will be specified with 0.1 μs resolution over its entire range of values. Entering [SPCL] [7] [5] [9] displays the current pulse width in the FREQUENCY display field with 0.1 μs resolution followed by a question mark prompt which indicates that a new pulse width can be entered. The characters "μS" are displayed in the AMPLITUDE display field to clarify that this is the pulse width entry even though it is displayed in the FREQUENCY display field. If the entered pulse width is longer than the pulse period (1 / Mod Frequency), the STATUS annunciator is flashed, and the pulse width is set to 0.1 μs less than the pulse period.

PULSE WIDTH

RANGE	RESOLUTION
0.1 us to 99.9999 ms	0.1 μs

SYNTAX:

[SPCL] [7] [5] [9] -- numeric data -- [MHz/V] [kHz/mV] [Hz/μV]

NOTE

The pulse width is always displayed with microsecond units. Pulse width entries are terminated with one of the following:

microsecond units = [MHz/V]
millisecond units = [kHz/mV]
second units = [Hz/μV]

EXAMPLE: Program a pulse width of 100.0 μs

FRONT PANEL: Enter [SPCL] [7] [5] [9]

The current pulse width is displayed in the FREQUENCY display field with a question mark prompt.

10 0000 ? US (current setting is 10000.0 μs)

Enter [1] [0] [0] [MHz/V] to program a 100 microsecond pulse width.

REMOTE: PULSE_WIDTH 100 US

Section 4D
Instrument State Memory

ORGANIZATION OF INSTRUMENT STATE MEMORY 4D-1.

The Signal Generator features non-volatile memory for storage and recall of instrument settings. Up to 50 full instrument settings can be saved and recalled through memory operations. Six different memory operations are allowed from the front panel:

- Recall of a memory location
- Store to a memory location
- Recall next memory location
- Recall previous memory location
- Store a single function parameter.
- Recall a single function parameter.

All except the single function store and recall are available in remote. The contents of non-volatile memory are preserved for at least 2 years with the Signal Generator's power off. Whenever you turn off the power, memory location 00 always saves the last instrument settings.

Each memory location contains all of the commonly accessed parameters needed to program the Signal Generator. However, the rf on/off state is unaffected by memory recall operations. Certain other parameters are also not storable or recallable. These parameters are described in the Table 4D-1.

The non-volatile memory locations are organized as shown in Table 4D-2.

Table 4D-1. Non-Storable/Recallable Parameters

PARAMETER CATEGORY	PARAMETER
IEEE	Address Talk-Only/Listen-Only/Addressed Mode Language Service Request Enable Event Status Enable Instrument Status Change Enable Device Trigger Buffer Protected User Data
MEMORY	Dividers Memory Lock State
MISCELLANEOUS	RF ON/OFF state Alternate External Reference Frequency Output Correction Display ON/OFF state Key Repeat Rate State

Table 4D-2. Non-volatile Memory Locations

LOCATIONS	DESCRIPTIONS
00	A scratch pad location that is a copy of the last valid instrument state before a memory, store, or recall operation. On power-on, it contains the instrument state when the power was turned off. If the last memory operation was store, location 00 contains the instrument state in the memory location that was written by the store operation. If the last memory operation was a recall or sequence, location 00 contains the instrument state before the recall operation. The entry [RCL] [0] [0] can be thought of as an "undo" command for memory operations.
01-50	Available for storage and recall of preset states of the Signal Generator.
51-95	Not used.
96	Holds the single parameter store and recall values. See the heading "Single Parameter Store and Recall" in this Section.
97	The Signal Generator Default Memory Location. All memory locations can be initialized to this setting with a Special Function command. See Section 4F, "Special Functions" for more information. The Instrument Preset State is presented in Appendix A.
98	Diagnostic instrument state.
99	The current instrument state.

STORING AND RECALLING INSTRUMENT STATES 4D-2.

Storage and recall of Signal Generator instrument states in non-volatile memory locations is accomplished with the [STO] and [RCL] keys. Note that memory store and recall operations perform no action while digital sweep is active.

SYNTAX:

Storing a Signal Generator Instrument State

1. The current instrument state is stored by pressing the [STO] key.

The last memory location stored or recalled is displayed in the FREQUENCY display field.

2. The DATA keys are used to enter the two-digit memory location code. The entered code must contain both digits (e.g., 01, 02, ...50).

The location code appears in the FREQUENCY display field as it is entered. When the second digit key of the location code is released, the store operation is performed. From Remote, the *SAV command is used to store an instrument state.

Recalling a Signal Generator Instrument State

1. An instrument state is recalled by pressing the [RCL] key. The last memory location stored or recalled is displayed in the FREQUENCY display field.

2. Use the DATA keys to enter the memory location code of the desired instrument state. Again, the entered code must contain both digits of the two-digit memory location code. When the second digit key of the location code is released, the recall operation is performed. From Remote, the *RCL command is used to recall an instrument state.

EXAMPLE: Recall the default memory location (97), program the RF Frequency to 6 MHz, and store it in memory location 06.

FRONT PANEL: [RCL] [9] [7] [FREQ] [6] [MHz/V] [STO] [0] [6]

REMOTE: *RCL 97; FREQ 6 MHZ; *SAV 6

RECALLING A SEQUENCE OF INSTRUMENT STATES 4D-3.

The following information describes the method for sequencing through memory locations containing the Signal Generator instrument states. Note that memory sequence operations perform no action while any digital sweep is active.

1. The [SEQ] key allows the stored instrument states to be sequentially recalled. The sequence operation recalls the next higher memory location, starting from the most recent memory location stored or recalled. When the highest location is reached, the sequence starts over again at location 01. in remote, the SEQ UP command accomplishes the same result.

2. While [SEQ] is pressed, the next memory location number is displayed and the memory location is recalled. While this key is pressed, the function continues to sequence up through through memory locations.

3. The previous memory location may be recalled by entering [RCL] [—] . This is equivalent to a sequence down function. While the [—] key is pressed, the function continues to sequence down through memory. The sequence down function "wraps" just as the sequence up function does. Entering [RCL] [—] when the last location was location 01 recalls the highest available memory location. in remote, the SEQ DOWN command accomplishes the same result.

DIVIDING MEMORY INTO PARTITIONS 4D-4.

Memory sequence dividers can be defined that partition the 50 memory locations into multiple subsets for sequence operations. Once defined, a memory divider sets an upper bound for sequence up operations and a lower bound for sequence down operations. From the front panel, the dividers are defined with a Special Function command; in remote, they are defined with the MEM_DIVIDER command.

If no dividers have been defined, the sequence up operation sequences through every location and wraps around at location 50 back to location 01. The sequence down operation sequences down through every location and wraps around at location 01.

If, for example, a divider is defined at location 10, the memory locations are partitioned into two subsets (1-9 and 10-50). Note that the memory location corresponding to the divider location is included in the upper subset and is excluded from the lower subset.

Up to four memory dividers can be defined at once. Locations 01 and 50 are always used as the absolute boundaries regardless of the divider settings. Therefore, four dividers can provide up to five memory location subsets.

Entering [SPCL] [8] [0] [2] displays the current memory divider settings. The settings of all four of the dividers are displayed at once. Inactive dividers are displayed as location 00. If a numeric key is pressed while the divider settings are displayed, it is interpreted as a new divider entry, and the Signal Generator enters the memory divider entry mode.

Once in the memory divider entry mode, the Signal Generator expects settings for all four dividers to be entered before any are updated. Only numeric keys and the [.] key are allowed. All other keys immediately exit the entry mode and all partial entries are discarded. The [.] key skips to the next divider entry (if no partial entry has been made) to simplify the entry process if some of the dividers are to be changed but others are to be left unchanged. A divider is deleted when its location is specified as 00.

After all four divider settings have been updated, the entries are sorted and redisplayed for five seconds. The following example illustrates the memory divider setting display and the memory divider entry mode.

EXAMPLE: Current divider settings are 00, 00, 07, 22. Change the divider settings to 00, 07, 14, 31.

FRONT PANEL:

Enter [SPCL] [8] [0] [2]. The display shows:

00 00 07 22

To change divider #1 from 00 to 14 (entries will be sorted automatically), enter [1]. The display shows:

d1 1_ ?

Enter [4] to complete the entry. The display then shows divider #2:

d2 00 ?

Only three dividers are in use, so enter [.]. The display then shows divider #3:

d3 07 ?

Leave this divider set to 07 by entering [.] again. The display then shows divider #4.

d4 22 ?

Enter [3]. The display shows:

d4 3_ ?

Enter [1]. The display shows:

d4 31 ?

When the [1] key is released, the new divider settings are sorted and the display shows for five seconds:

00 07 14 31

Note that location 07 has moved from divider #3 to divider #2. Since the dividers are kept sorted, the actual divider number is not particularly important. However, the divider numbers do provide a way to uniquely identify each divider.

REMOTE: MEM_DIVIDER 00,07,14,31

From the front panel, divider entries that are out of range are immediately rejected. To enter a valid divider following an erroneous entry, the entry process must be started over from the beginning. Duplicate divider entries are not checked as they are entered, but are eliminated during the sorting process.

WRITE-PROTECTING MEMORY LOCATIONS 4D-5.

Memory locations 01 through 50 and 96 can be write-protected with a Special Function command from the front panel, or with the MEM_LOCK command in remote. When enabled, all memory recall and sequence operations operate as usual, but memory store operations are rejected.

SYNTAX:

	FRONT PANEL	REMOTE
Disable Memory Lock	SPCL 8 1 0	MEM_LOCK OFF
Enable Memory Lock	SPCL 8 1 1	MEM_LOCK ON

RESETTING ALL MEMORY LOCATIONS TO FACTORY DEFAULT 4D-6.

The contents of the 50 non-volatile memory locations and memory locations 96 and 99 can be reset to the default memory location (97) with a Special Function command from the front panel as described below. (Memory location 97 is described in Appendix A, "Instrument Preset State".)

1. Entering SPCL 8 0 1 from the front panel, or sending the Remote command MEM_RESET causes the message "Sto ?" to appear in the FREQUENCY display field.

2. If the STO key is pressed within 10 seconds, the memory contents are reset to the memory location default (97).

3. If the STO key is not pressed within 10 seconds, or if any other key is pressed, memory locations will not be changed.

STORING AND RECALLING SINGLE PARAMETERS 4D-7.

A single function parameter may be stored or recalled individually without affecting the entire instrument state. This allows individual storage and recall of commonly used rf output frequency, rf amplitude, AM depth, FM/ϕM deviation, modulation frequency and modulation level parameter values. The stored parameters are saved in memory location 96. This location is initialized to the instrument default state if no parameters have been stored.

Pressing the STO key followed by a FUNCTION key stores the current value of the function parameter for later use. Pressing the RCL key followed by a FUNCTION key recalls only the specified parameter leaving all other Signal Generator parameters unchanged. For example, entering STO FREQ saves the current rf output frequency. Entering RCL FREQ recalls the parameter value without affecting any other programmed functions.

The rf output frequency store and recall operations preserve the state of Relative Frequency Mode along with the offset and the reference value. Likewise, the rf amplitude store and recall operations preserve the state of Relative Amplitude Mode along with the offset and the reference value.

Section 4E
Sweep

INTRODUCTION 4E-1.

The Signal Generator provides digital sweep capability for both rf output frequency and rf amplitude. Each has three modes of operation: auto sweep, manual sweep, and single sweep.

Auto digital sweep mode cycles continuously through the sweep range, with a selected dwell time at each discrete frequency or amplitude. The display reflects the center frequency or amplitude; the bright digit remains on. All numeric function entries are allowed while auto sweep is active.

Manual digital sweep mode increments and decrements within the sweep range with the edit knob, in units of the sweep increment. The display reflects the output (relative mode off) or offset (relative mode on) frequency or amplitude. The display bright digit is turned off, and any key entry that relies on the position of the bright digit is disallowed. This includes function selection, numeric entry, and units entry. All other front panel keys are allowed.

Single digital sweep mode runs through the sweep range once, with a selected dwell time at each discrete frequency or amplitude. The display is continuously updated to reflect the output (relative mode off) or offset (relative mode on) frequency or amplitude, with the bright digit off. Only the RF OUTPUT [ON/OFF], [STATUS], [AUTO] and [MANUAL] keys are active.

When any mode of digital sweep is active, a 0 to 10V stepped output ramp is available at the rear panel AUX connector. This signal is an analog of the progress of the sweep. A TTL-level pulse is available on this connector for X-Y recorder pen lift control or for oscilloscope Z-axis blanking. When an auto or single sweep reaches the end of its range, the signal is driven high for a 100 millisecond (minimum) pulse. See Appendix F for the AUX connector pinout diagram.

In all sweep modes, memory store and recall operations (the [STO], [RCL], and [SEQ] keys) are disallowed. If the Signal Generator is powered off while any sweep is active, the active sweep is terminated, and the power-down memory location (location 00) is programmed to the center frequency or amplitude.

SELECTING FREQUENCY OR AMPLITUDE SWEEP 4E-2.

Selection of frequency sweep or amplitude sweep from the front panel is performed by pressing the desired function key, followed by either sweep parameter. No numeric entry or unit entry is necessary to change the sweep field. The SWEEP_FIELD command selects the desired function from Remote. The selected function has the SWP annunciator lit in its display field. This operation ties the selected function (frequency or amplitude) to the sweep mode controls, but does not activate any of the sweep modes (auto, manual, or single). The sweep field may not be changed while a sweep is active.

SYNTAX:

	FRONT PANEL	REMOTE
Select Frequency Sweep	FREQ SWEEP WIDTH or FREQ SWEEP INCR	SWEEP_FIELD FREQ
Select Amplitude Sweep	AMPL SWEEP WIDTH or AMPL SWEEP INCR	SWEEP_FIELD AMPL

SUMMARY OF SWEEP MODES 4E-3.

From the front panel, Auto and Manual Sweep Mode are enabled and disabled by pressing keys located in the SWEEP ON/OFF section, while Single Sweep is enabled with a Special Function command. in remote, the SWEEP command selects a Sweep Mode.

The sweep on/off keys operate as toggle functions; the key enables a sweep mode is pressed again to disable the mode. For example, pressing the AUTO key once enables the auto sweep mode and pressing the AUTO key again turns off the auto sweep. The same holds true for the MANUAL key. Since the single sweep mode is enabled by Special Function and terminates automatically, no direct toggle capability is provided. However, pressing either the AUTO or MANUAL key twice terminates a single sweep. From Remote, the SWEEP OFF command turns off any active sweep.

If MANUAL is pressed while a single or auto sweep is active, the manual sweep mode is entered precisely at the point in the sweep range where the Signal Generator was at the time the key was pressed. This allows the neighborhood of a particular frequency or amplitude in the sweep range to be examined in greater detail. If AUTO is pressed again, the sweep resumes from the last point where it was left in the manual sweep.

SYNTAX:

	FRONT PANEL	REMOTE
Initiate Auto Sweep	AUTO	SWEEP AUTO
Initiate Manual Sweep	MANUAL	SWEEP MANUAL
Initiate Single Sweep	SPCL 8 8 2	SWEEP SINGLE
Terminate Sweep	AUTO if AUTO on MANUAL if MANUAL on	SWEEP OFF

SELECTING SYMMETRIC OR ASYMMETRIC SWEEP 4E-4.

Both symmetric (sweep range is evenly centered about displayed frequency or amplitude) and asymmetric sweep (displayed frequency or amplitude is an endpoint of the sweep range) are selectable with a Special Function command from the front panel. in remote, the SWEEP_SYM command is used. When asymmetric sweep is selected the ASYM annunciator is lit. If a selection is made that would cause an invalid sweep range while a sweep is active, the entry is rejected.

SYNTAX:

	FRONT PANEL	REMOTE
Select Symmetric Sweep	SPCL 8 8 0	SWEEP_SYM SYMM
Select Asymmetric Sweep	SPCL 8 8 1	SWEEP_SYM ASYM

SETTING SWEEP DWELL TIME 4E-5.

The time that an active auto or single sweep dwells at each discrete frequency or amplitude in the sweep range can be adjusted. This dwell time is in addition to the nominal switching time for frequency and amplitude. One of six different minimum dwell times can be selected with a Special Function command from the front panel, or with the SWEEP_DWELL command in remote. The selected dwell time remains in effect for all subsequent sweep modes.

SYNTAX:

	FRONT PANEL	REMOTE
Select 0 ms Dwell	SPCL 8 9 0	SWEEP_DWELL 0 MS
Select 20 ms Dwell	SPCL 8 9 1	SWEEP_DWELL 20 MS
Select 50 ms Dwell	SPCL 8 9 2	SWEEP_DWELL 50 MS
Select 100 ms Dwell	SPCL 8 9 3	SWEEP_DWELL 100 MS
Select 200 ms Dwell	SPCL 8 9 4	SWEEP_DWELL 200 MS
Select 500 ms Dwell	SPCL 8 9 5	SWEEP_DWELL 500 MS

FREQUENCY SWEEP

4E-6.

The Signal Generator allows digital frequency sweep between any two valid frequencies with a resolution of 1 Hz per increment.

Four parameters define the sweep:

- The rf output frequency in effect before the sweep is enabled becomes the center frequency if symmetric sweep is selected, or the start frequency if asymmetric sweep is selected. It is generically called the center frequency (Fc).
- The frequency sweep width (Fw) is the total width of the sweep and may be either a positive or a negative quantity.
- The frequency sweep increment (Fi) is the increment size and must be a positive quantity. The sweep increment may be larger than the absolute value of the sweep width.
- Sweep symmetry is selected by Special Function, as described in the under the heading "Digital Sweep Symmetry".

The following equations show the relationship of these parameters.

NOTE

The progression of the sweep is always from F1 to F2. (Fw can be negative.)

Symmetric sweep: ASYM annunciator is off.

F1 = start frequency = Fc - Fw/2

F2 = end frequency = Fc + Fw/2

Asymmetric sweep: ASYM annunciator is lit.

F1 = start frequency = Fc

F2 = end frequency = Fc + Fw

Some sweep parameters may be changed while sweep is active. Any parameter change that would result in an invalid sweep condition is rejected, and the sweep continues with the existing sweep parameters. If an attempt is made to start a sweep with such a combination of parameters, the sweep mode selection is rejected.

During auto sweep, both sweep width and sweep increment can be inspected and modified, and the center frequency can be modified, edited, or stepped. If the entry is valid, the new sweep range or increment takes effect immediately for the sweep. These parameters cannot be displayed or changed during manual or single sweep, although the center frequency may be stepped during manual sweep. Sweep symmetry may be changed at any time (so long as the resulting sweep range is valid) for auto or manual sweep. Sweep symmetry may not be changed while a single sweep is active.

A sweep in relative mode is possible by enabling relative frequency mode before entering a sweep. However, relative mode may not be enabled or disabled while a sweep is active.

Setting Frequency Sweep Width 4E-7.

The frequency sweep width can be selected for entry by first pressing the [FREQ] key to select the FREQUENCY display field, then pressing the [SWEEP WIDTH] key. Upon programming a new sweep width, the value is held momentarily in the FREQUENCY display field. A negative sweep width can be entered; this causes the Signal Generator to sweep in the reverse direction, that is, starting at the high frequency and proceeding towards the low frequency.

FREQUENCY SWEEP WIDTH

	RANGE	RESOLUTION
6080A	±1 to ±1056 MHz	1 Hz
6082A	±1 to ± 2112 MHz	1Hz

SYNTAX:

[FREQ] [SWEEP WIDTH] -- numeric data -- [MHz|V] [kHz|mV] [Hz|µV]

EXAMPLE: Set Frequency Sweep Width to 230 MHz

FRONT PANEL: [FREQ] [SWEEP WIDTH] [2] [3] [0] [MHz|V]

REMOTE: FREQ_SWIDTH 230 MHZ

Setting Frequency Sweep Increment 4E-8.

The frequency sweep increment can be selected for entry by first pressing the [FREQ] key, to select the FREQUENCY display field, then pressing the [SWEEP INCR] key. Upon programming a new sweep increment, the new value is held momentarily in the FREQUENCY display field.

FREQUENCY SWEEP INCREMENT

	RANGE	RESOLUTION
6080A	1 to 1056 MHz	1 Hz
6082A	1 to 2112 MHz	1Hz

SYNTAX:

[FREQ] [SWEEP INCR] -- numeric data -- [MHz|V] [kHz|mV] [Hz|µV]

EXAMPLE: Set Frequency Sweep Increment to 230 MHz

FRONT PANEL: [FREQ] [SWEEP INCR] [2] [3] [0] [MHz|V]

REMOTE: FREQ_SINCR 230 MHZ

Digital Frequency Sweep Example 4E-9.

EXAMPLE: Configure a digital frequency sweep From 500 MHz to 540 MHz, with a sweep increment of 100 kHz and a dwell of 0 ms at each point. Enable Single sweep for this configuration.

1. Select 520 MHz RF frequency

FRONT PANEL: [FREQ] [5] [2] [0] [MHz/V]

REMOTE: FREQ 520 MHZ

2. Select 40 MHz frequency sweep width and select frequency as the active sweep field

FRONT PANEL: [FREQ] [SWEEP WIDTH] [4] [0] [MHz/V]

REMOTE: FREQ_SWIDTH 40 MHZ ; SWEEP_FIELD FREQ

3. Select 100 kHz frequency sweep increment

FRONT PANEL: [FREQ] [SWEEP INCR] [0] [.] [1] [MHz/V]

REMOTE: FREQ_SINCR 0.1 MHZ

4. Select symmetric sweep

FRONT PANEL: [SPCL] [8] [8] [0]

REMOTE: SWEEP_SYM SYMM

5. Select 0 ms sweep dwell time

FRONT PANEL: [SPCL] [8] [9] [0]

REMOTE: SWEEP_DWELL 0 MS

6. Enable single sweep

FRONT PANEL: [SPCL] [8] [8] [2]

REMOTE: SWEEP SINGLE

AMPLITUDE SWEEP 4E-10.

The Signal Generator allows both digital linear and digital logarithmic amplitude sweep. If all amplitude sweep parameters are specified in linear (voltage) quantities, the sweep will be digital linear. If all amplitude sweep parameters are specified in logarithmic (dBm, dBmV, dBμV or dBf) quantities, the sweep will be digital logarithmic.

Four parameters define the sweep:

- The rf amplitude in effect before the sweep is enabled becomes the Center Amplitude if symmetric sweep is selected, or the start amplitude if asymmetric sweep is selected. It is generically called the Center Amplitude (Ac).

- The amplitude sweep width (Aw) is the total width of the sweep and may be either a positive or a negative quantity.

- The amplitude sweep increment (Ai) is the increment size and must be a positive quantity. The sweep increment may be larger than the absolute value of the sweep width.

- Sweep symmetry is selected by Special Function.

The following equations show the relationship of these parameters.

NOTE

The progression of the sweep is always from A1 to A2. "Aw" can be negative.

Symmetric sweep: ASYM annunciator is off.

A1 = start amplitude = Ac - Aw/2

A2 = end amplitude = Ac + Aw/2

Asymmetric sweep: ASYM annunciator is lit.

A1 = start amplitude = Ac

A2 = end amplitude = Ac + Aw

Certain sweep parameters may be changed while sweep is active. Any parameter change that would result in an invalid sweep condition is rejected and the sweep continues with the existing sweep parameters. If an attempt is made to start a sweep with such a combination of parameters, the sweep mode selection is rejected.

During auto sweep, sweep width and sweep increment can be inspected and modified, the center amplitude can be edited or stepped, and sweep symmetry may be changed. If the entry is valid, the new sweep range or increment takes effect immediately. With the exception of stepping the center amplitude during manual sweep, these parameters cannot be displayed or changed during manual or single sweep.

The center amplitude, sweep width, and sweep increment must all have consistent units (dB or volts). If these parameters have inconsistent units, the amplitude sweep will be rejected when a sweep mode (auto, manual, or single) is enabled. Likewise, the units of the sweep parameters may not be converted while amplitude sweep is active.

A sweep in relative mode is possible by enabling relative amplitude mode before entering a sweep. However, relative mode may not be enabled or disabled while a sweep is active.

The maximum sweep width in either logarithmic or linear mode is restricted to 20 dB (approximately a 10:1 ratio). Furthermore, when in linear mode, the ratio of the maximum output voltage in the amplitude sweep to the sweep increment cannot exceed 999.

Setting Amplitude Sweep Width 4E-11.

The amplitude sweep width can be selected for entry by first pressing the AMPL key to select the AMPLITUDE display field, then pressing the SWEEP WIDTH key. When a new sweep width is programmed, the value is held momentarily in the AMPLITUDE display field. A negative sweep width can be entered; this causes the Signal Generator to sweep in the reverse direction, that is, starting at the larger amplitude and proceeding towards the smaller amplitude.

AMPLITUDE SWEEP WIDTH

RANGE	RESOLUTION
± 0.1 dB to ±20 dB ±10 nV to ±2.24 V	0.1 dB 3 digits

SYNTAX:

AMPL SWEEP WIDTH -- numeric data -- dB(m) / MHz/V / kHz/mV / Hz/µV

EXAMPLE: Set Amplitude Sweep Width to 12 dB

FRONT PANEL: AMPL SWEEP WIDTH 1 2 dB(m)

REMOTE: AMPL_SWIDTH 12 DB

Setting Amplitude Sweep Increment 4E-12.

The amplitude sweep increment can be selected for entry by first pressing the AMPL key to select the AMPLITUDE display field, then pressing the SWEEP INCR key. Upon programming a new sweep increment, the new value is held momentarily in the AMPLITUDE display field.

AMPLITUDE SWEEP INCREMENT

RANGE	RESOLUTION
0.1 to +20 dB 10 nV to 2.24 V	0.1 dB 3 digits

SYNTAX:

AMPL SWEEP INCR -- numeric data -- dB(m) / MHz/V / kHz/mV / Hz/µV

EXAMPLE: Set amplitude sweep increment to 0.5 dB

FRONT PANEL: AMPL SWEEP INCR 0 . 5 dB(m)

REMOTE: AMPL_SINCR 0.5 DB

Digital Amplitude Sweep Example 4E-13.

EXAMPLE: Configure a digital amplitude sweep from -20.0 dBm to -15.0 dBm, with a sweep increment of 0.1 dB and a dwell of 100 ms at each point. Enable Auto sweep for this configuration.

1. Select -20.0 dbm RF amplitude

FRONT PANEL: [AMPL] [—] [2] [0] [dB(m)]

REMOTE: AMPL -20 DBM

2. Select 5 dB amplitude sweep width and select amplitude as the active sweep field

FRONT PANEL: [AMPL] [SWEEP WIDTH] [5] [dB(m)]

REMOTE: AMPL_SWIDTH 5 DB ; SWEEP_FIELD AMPL

3. Select 0.1 dB amplitude sweep increment

FRONT PANEL: [AMPL] [SWEEP INCR] [0] [.] [1] [dB(m)]

REMOTE: AMPL_SINCR 0.1 DB

4. Select asymmetric sweep

FRONT PANEL: [SPCL] [8] [8] [1]

REMOTE: SWEEP_SYM ASYM

5. Select 100 ms sweep swell time

FRONT PANEL: [SPCL] [8] [9] [3]

REMOTE: SWEEP_DWELL 100 MS

6. Enable auto sweep

FRONT PANEL: [AUTO]

REMOTE: SWEEP AUTO

CALIBRATING A RECORDER OR OSCILLOSCOPE 4E-14.

To calibrate an X-Y plotter/recorder or oscilloscope to the Signal Generator X-axis (sweep DAC) output and the blanking/pen lift signals, use the following procedure:

1. Set the X-axis output to 0 volts:

   Enable manual sweep and turn the edit knob to the start frequency (F1) or the start amplitude (A1).

2. Set the X-axis output to +10 volts:

   Enable manual sweep and turn the edit knob to the end frequency (F2) or the end amplitude (A2).

The blanking/pen lift signal is maintained "low" for the above conditions; it is maintained "high" if no sweep is active.

ANALOG FREQUENCY SWEEP 4E-15.

It is possible to configure the Signal Generator FM circuitry to perform a fast frequency sweep that is symmetric about the rf output frequency. This mode is entirely controlled by the programmed modulation parameters and is not related to the synthesized digital sweep.

Three parameters must be configured to perform a fast frequency sweep:

- The sweep rate, determined by the modulation frequency.

  At lower modulation frequencies, it may be necessary to enable Low Rate FM or External DC FM. See Section 4C, "Modulation" for more information.

- The programmed FM deviation (one-half of the sweep width).

  The maximum FM deviation allowed depends on the rf output frequency. See Section 4C, "Modulation" for more information.

  The following equations determine the start and end frequencies:

  F1 = start frequency = rf output frequency - FM deviation

  F2 = end frequency = rf output frequency + FM deviation.

- The triangle internal modulation waveform must be selected.

  See Section 4C, "Modulation" for more information.

Once internal FM is enabled, the rf output frequency sweeps from F1 to F2, then back down to F1 each period (period = 1/Modulation Frequency).

EXAMPLE: Configure an analog frequency sweep from 199.5 MHz to 200.5 MHz, with a sweep rate of 100 Hz.

1. Select 200-MHz rf frequency

FRONT PANEL: [FREQ] [2] [0] [0] [MHz|V]

REMOTE: FREQ 200 MHz

2. Select 100-Hz modulation frequency

FRONT PANEL: [MOD FREQ] [1] [0] [0] [Hz|µV]

REMOTE: MODF 100 Hz

3. Select 1 MHz FM deviation

FRONT PANEL: [FM|øM] [1] [MHz|V]

REMOTE: FM 1 MHz

4. Select triangle internal modulation waveform

FRONT PANEL: [SPCL] [7] [5] [1]

REMOTE: MOD_WAVE TRIANGLE

5. Enable internal FM modulation

FRONT PANEL: [INT FM|øM]

REMOTE: INT_FM ON

Section 4F
Special Functions

INTRODUCTION 4F-1.

Special Functions are divided into three functional groups:

- Stored-mode
- Immediate action
- Hidden parameter display/entry.

All are activated by pressing the [SPCL] key followed by either a two- or three-digit numeric code.

Stored-mode Special Functions change a specific operating mode of the Signal Generator. Examples are rf output frequency Relative mode, Low-rate FM mode, and High-rate ϕM mode. All of the active stored-mode Special Function numeric codes can be viewed by pressing the [SPCL] key.

Each of the stored-mode Special Functional groups is allocated a decade of Special Function numeric codes. For example, Relative rf output frequency OFF/ON is 20/21, low-rate FM OFF/ON is 710/711, and High-rate ϕM OFF/ON is 720/721. The unit digit of the code determines whether functions of this type are off or on (0 = OFF, 1 =ON). The Signal Generator's default, preset state forces these functions to the OFF state, except for the display, which is on by default.

All enabled stored-mode functions are cleared with Special Function 00.

Some of the stored-mode functions have more than two choices. For example, there are six selections (890 through 895) for sweep dwell time, and three selections (750 through 752) for the internal modulation waveform. Again, the unit digit of the code determines the selection within the decade, with the zero-state the default state.

Immediate action Special Functions typically perform an immediate action without affecting the stored state of the Signal Generator. Examples of these type of functions include display of the software revision level and execution of self-tests. Since immediate action functions do not change the stored state of the Signal Generator, their Special Function numbers are not allocated in decades.

Hidden parameter Special Functions are for display and modification of Signal Generator parameters that are not normally displayed on the front panel. Hidden parameter Special Functions are used primarily when the related parameter may take on a wide range of values and it is impractical to use a sequence of Special Function

numbers. Since the Special Function number is not used as an indication of the function state, they are not allocated in decades. An example of this type of function is Special Function 10, which displays and sets the IEEE-488 address.

Table 4F-1 lists the Special Functions by action. Appendix B contains a list of the Special Function codes.

Table 4F-1. Special Function Codes

SPECIAL FUNCTION DESCRIPTION	FRONT PANEL	REMOTE COMMAND	LIGHTS SPCL ANNUNCIATOR WHEN ENABLED
FREQUENCY			
Relative frequency mode	20,21	FREQ_REL	
Enable phase adjustment	701	PHASE	
Zero phase adjustment	702	PHASE_ZERO	
External reference input frequency	760,761	EXTREF_FREQ	
AMPLITUDE			
Relative amplitude mode	30,31	AMPL_REL	
Fixed-range amplitude	50,51	AMPL_RANGE	*
Amplitude display units	840-843	AMPL	
EMF-Volts amplitude display mode	850,851	AMPL_EMFOUT	
MODULATION			
Modulation oscillator output	40,41	MODOUT	*
Enter modulation frequency to 0.1 Hz	42	MODF	
Low-rate FM	710,711	LORATEFM	*
High-rate ØM	720,721	HIRATEPM	*
Low-distortion/fixed-range FM	730-732	FM_RANGE	*
Internal pulse modulation	740,741	INT_PULSE	
Modulation oscillator waveform	750-752, 758	MOD_WAVE	*
Enter pulse width	759	PULSE_WIDTH	
SWEEP			
Sweep dwell time	890-895	SWEEP_DWELL	
Sweep symmetry	880,881	SWEEP_SYM	
Initiate single sweep	882	SWEEP SINGLE	
INSTRUMENT STATE MEMORY			
Reset memory locations	801	MEM_RESET	
Display/Set memory sequence dividers	802	MEM_DIVIDER	
Write-protect memory locations	810,811	MEM_LOCK	
REMOTE			
Display/Set IEEE-488 address	10	n/a	
Display/Set IEEE-488 address mode	11	n/a	
Display/Set IEEE-488 language	12	GAL	
Display/Enter service request mask	13	*SRE	
Set user request SRQ	14	n/a	
Clear SRQ	15	n/a	

Table 4F-1. Special Function Codes (cont)

SPECIAL FUNCTION DESCRIPTION	FRONT PANEL	REMOTE COMMAND	LIGHTS SPCL ANNUNCIATOR WHEN ENABLED
MISCELLANEOUS			
Clear special functions	00	SPCL 00	
Restore Instrument Preset State	01	SPCL 01	
Initiate power-on self tests	02	*TST?	
Display self test results	03	STATUS	
Display option loading status	08	*IDN?	
Display software revision level	09	*IDN?	
Disable display	770,771	DISPLAY	
Step key repeat rate	860-862	KEY_RATE	
Knob and step key operation	870-873	KNOB_STEP	*
SERVICE			
Amplitude compensation	920-922	AMPL_COMP	*
Output compensation data	930,931	AMPL_CMPDAT	
See Service Manual for Others			

ENABLING SPECIAL FUNCTIONS 4F-2.

The Special Function code is a two or three digit number. Special Functions 00 through 19 cause an immediate action to be performed. Special functions 20 through 59 and 600 through 999 cause a change to the instrument state. The first digit indicates the classification of the Special Function, and the last digit specifies the particular Special Function. A Special Function is executed when the last digit of the Special Function code is entered.

SYNTAX:

<n> = 0..9:

Special Functions 00 through 59 [SPCL] <n> <n>

Special Functions 600 through 999 [SPCL] <n> <n> <n>

VIEWING ENABLED SPECIAL FUNCTIONS 4F-3.

A list of the active stored-mode Special Functions is displayed while the [SPCL] key is pressed. A Special Function is defined as active, and its code is displayed, only when it is programmed to a state other than its default state. If all Special Functions are in their default or OFF state, the code 00 is displayed.

Up to four Special Function codes are displayed at a time. If more than four Special Functions are active, repeatedly pressing the [SPCL] key scrolls through the list. For more information on the operation of the Special Function status display, see Section 4G, "Error and Status Reporting".

THE SPCL ANNUNCIATOR 4F-4.

Several Special Functions enable operating modes that cause a distinct change to the state of the Signal Generator, but do not have a dedicated annunciator in the display. The SPCL annunciator in the FREQUENCY display field is lit when any of these special operating modes are enabled.

In addition, the SPCL annunciator is lit for Special Functions for which there is a dedicated annunciator, but are context dependent. For example, enabling the low-rate FM Special Function lights the SPCL annunciator immediately, but the LO RATE annunciator is lit only if Internal or External FM is also enabled.

MISCELLANEOUS SPECIAL FUNCTIONS 4F-5.

Disable Special Functions 4F-6.

Enabled stored-mode Special Functions can be cleared with Special Function 00.

Restore Instrument Preset State 4F-7.

Enabled stored-mode Special Functions can also be cleared with Special Function 01. This function recalls memory location 97 clears all sweep modes and cal/comp procedures. The scope of Special Function 01 is detailed in Appendix A.

Execute Self-Test and Display Self-Test Results 4F-8.

The Signal Generator performs self-tests of its digital and analog hardware at power-on or by Special Function. Self-tests can be run at any time with Special Function 02.

The test sequence can be terminated immediately by pressing any front panel key. At the end of the test sequence, the Signal Generator assumes the power-on-state. Numeric error codes are displayed if one or more of the self tests failed. If the tests were aborted with a key entry, error code 301 is displayed to indicate that the tests were not run to completion.

The results of the self-tests can be displayed with Special Function 03. See Appendix E for the status codes and their explanations.

For safety (for example where an amplifier is attached to the Signal Generator), self tests are run without energizing the rf output. To run self-tests that include energizing the rf output, use Special Function 06.

Display Loaded Options 4F-9.

Special Function 08 causes the loaded instrument options to be displayed for approximately 5 seconds or until another key is pressed.

Display Instrument ID and Software Revision Level 4F-10.

Special Function 09 causes the instrument ID and software revision level to be displayed in the display fields for approximately 5 seconds or until another key is pressed.

Blank Front Panel Display 4F-11.

The front panel display can be blanked with Special Function 771. This Special Function blanks the display and disables the edit knob. Special Function 770 restores the display and functionality of the knob.

Select Repeat Rate for Step Keys 4F-12.

The repeat rate for the front panel step [△] and [▽] keys is selected with Special Functions 860 through 862. The default repeat rate for the step keys is medium, corresponding to Special Function 860. Special Function 861 selects a fast repeat rate, while Special Function 862 selects a slow repeat rate.

Configure Edit Knob and Step Keys 4F-13.

The front panel edit knob can be disabled and the functional role of the step increment/decrement keys and the edit knob can be modified with Special Functions 871 through 873 (see Table 4F-2). With Special Function 871, the bright digit remains displayed even though edit operations are disabled.

Table 4F-2. Functions of Edit Knob and Step Keys

SPECIAL FUNCTION KEYS	EDIT KNOB	STEP INCREMENT/DECREMENT
870	Enabled	Enabled as step
871	Disabled	Enabled as step
872	Enabled	Enabled as edit
873	Disabled	Enabled as edit

Section 4G
Error and Status Reporting

GENERAL DESCRIPTION 4G-1.

There are five types of status information that the Signal Generator generates:

- Rejected Entry Errors
- Instrument Overrange/Uncal Status
- Self-Test Status
- Calibration/Compensation Data Checksum Status
- Calibration/Compensation Data Origin Status

The rejected entry annunciator REJ ENTRY is flashed whenever a front panel or Remote entry is rejected. Numeric data in one of the display fields may also flash to indicate the rejected value. Any function key may be pressed to clear the flashing entry and the REJ ENTRY annunciator.

The STATUS annunciator is lit but not flashed to indicate when the Signal Generator is operating outside its specified performance range. If abnormal operation or aberrated output occurs, the STATUS annunciator is flashed to emphasize the severity of the problem.

Since there is never more than one rejected entry error at a time, rejected entry errors are always given precedence over the status codes. To avoid ambiguity, the STATUS annunciator is always turned off when the rejected entry annunciator is flashing.

The Self-Test Status and Calibration/Compensation Data Status are not presented in the normal operation of the Signal Generator. A Special Function command displays the active status codes for these conditions.

THE STATUS KEY 4G-2.

When the REJ ENTRY annunciator is flashing, pressing the [STATUS] key displays the Rejected Entry Error Code; when the STATUS annunciator is flashing or lit, pressing the [STATUS] key displays the Overrange or Uncal Status Codes. These codes provide detailed information on the nature of the rejected entry or status condition.

To avoid ambiguity, every Rejected Entry, Overrange/Uncal, Self-Test and Calibration Compensation memory condition has a unique status code. These codes are organized numerically to facilitate their interpretation, as shown in Table 4G-1.

A numeric list and explanation of all of the error and status codes is presented in Appendixes C, D, and E.

Table 4G-1. Interpreting Status Codes

ERROR/STATUS CODE	INTERPRETATION
00	No Errors or Status
01 to 199	Rejected Entry Errors
201 to 299	Instrument Overrange or Uncal Status
301 to 399	Self-Test Status
401 to 499	Calibration/Compensation Data Checksum Status
501 to 599	Calibration/Compensation Data Origin Status

When the front panel REJ ENTRY annunciator is flashing, pressing the [STATUS] key displays a numeric code, in the MODULATION display field, indicating the specific reason why the entry was rejected. in remote, the ERROR? command is used to query errors.

When the front panel STATUS annunciator is lit or flashing, pressing the [STATUS] key displays one or more numeric codes detailing the set of overrange or uncal conditions. in remote, the STATUS? command is used to query status.

Up to four codes can be displayed at a time. If more than four status codes are active, repeatedly pressing the [STATUS] key will scroll through the active codes. Only three codes at a time are displayed when the active list is scrolled through. Three dots appear in the fourth (rightmost) field to indicate that there are additional codes.

DISPLAYING SELF-TEST STATUS AND CALIBRATION/ COMPENSATION DATA 4G-3.

Self-Test, Calibration/Compensation Data Checksum, and Origin status codes can also be displayed. Each set of status codes are displayed with a Special Function and scrolled using the [STATUS] key like the overrange/uncal status codes. in remote, the STATUS command is used to load the status queue with the requested information, and the STATUS? command is used to query the status. The Calibration/Compensation Data Checksum and Origin Status codes are described in the Signal Generator Service Manual.

SYNTAX:

	FRONT PANEL	REMOTE
Display/Load Overrange /Uncal Status	[STATUS]	STATUS UNCAL STATUS?
Display/Load Self Test Status	[SPCL] [0] [3] [STATUS]	STATUS SELFTEST STATUS?
Display/Load Cal/Comp Data Checksum Status	[SPCL] [0] [4] [STATUS]	STATUS CHECKSUM STATUS?
Display/Load Cal/Comp Data Origin Status	[SPCL] [0] [5] [STATUS]	STATUS ORIGIN STATUS?

Section 5
Remote Operation

INTRODUCTION 5-1.

The Signal Generator operates directly from the front panel controls or under remote control of an instrument controller or computer. The following sections describe how to connect, configure, and operate the Signal Generator in the remote mode.

The Signal Generator is fully programmable for use on the IEEE Standard 488.1 interface bus (IEEE-488 bus). The interface also complies with supplemental standard IEEE-488.2. Devices connected to the bus in a system are designated as talkers, listeners, talker/listeners, or controllers. Under the remote control of an instrument controller such as the Fluke 1722A, the Signal Generator operates exclusively as a talker/listener on the IEEE-488 bus. This operation is described in Section 5A, "Remote Programming". The programming commands are listed in Section 5B, "Remote Command Tables".

For an introduction to the basics of the IEEE-488 interface bus, request Fluke Application Bulletin AB-36, "IEEE Standard 488-1978 Digital Interface for Programmable Instrumentation."

The Signal Generator can also be operated on the IEEE-488 bus without an instrument controller in a talk-only or listen-only mode. In this mode, two Signal Generators can be configured to track each other in operation. This mode is described in Section 5C, "Listen-Only/Talk-Only Operation".

The Signal Generator internal software includes compatibility languages for emulating Fluke Models 6060A, 6060B, 6061A, 6062A, 6070A, and 6071A, and Hewlett Packard Models 8642A or B. This capability allows substituting a 6080A or 6082A for one of the above instruments in an existing system, with no, or in some cases minor, software modifications. These compatibility languages are described in Section 5D, "Compatibility Languages".

SETTING UP THE IEEE-488 INTERFACE 5-2.

The Signal Generator is set at the Fluke factory to operate in the normal talker/listener mode. If the listen-only/talk-only modes or the compatibility languages are to be used, follow the setup procedures described in this section.

Address Setup Procedure 5-3.

Setting up the Signal Generator on the IEEE-488 bus requires only a choice of address and connection to a controller. The address is set at the Fluke factory to 2. To change the Signal Generator address, proceed as follows:

Enter [SPCL] [1] [0] to display the current IEEE-488 address. The address is shown in the FREQUENCY display field, and the talker/listener mode is shown in the AMPLITUDE display field. For example:

EXAMPLE	EXPLANATION
"Addr 01 ? "	Normal mode with address of 1
"Addr 12 ? to"	Talk-only mode, address is ignored
"Addr 23 ? Lo"	Listen-only mode, address is ignored

Enter two digits for the desired new address. Addresses are allowed in the range of 0 to 30. The new address is displayed for 2 seconds.

The address is stored in non-volatile memory and is retained when the power is turned off.

Talker/Listener Mode Selection Procedure 5-4.

When using an IEEE-488 bus controller, the Signal Generator should be set to operate in the addressed mode. A talk-only and listen-only mode are provided for use on the IEEE-488 bus without a controller. Two Signal Generators can be connected together to track each other with the talk-only and listen-only modes.

Enter [SPCL] [1] [1] to display the current talker/listener mode in the FREQUENCY display field.

EXAMPLE	EXPLANATION
Addr ?	Normal (Addressed) mode
to ?	Talk-only mode
Lo ?	Listen-only mode

When the Signal Generator is in talk-only or listen-only, it is always addressed to talk or listen, so the ADDR annunciator on the front panel is always lit.

Enter [0] to select the addressed mode, [1] to select the talk-only mode, and [2] to select the listen-only mode. The new talker/listener mode is displayed for 2 seconds.

The selected mode is stored in non-volatile memory and retained when the power is turned off.

Compatibility Language Selection Procedure 5-5.

The default language for the Signal Generator is described in this section. To select and use an alternate language for emulating a supported model of signal generator, refer to Section 5D.

If anything but the 6080 language is selected, the Signal Generator will not respond to the commands described in this section. See Section 5D for more information.

Verify that the default 6080 language is selected by entering [SPCL] [1] [2] to display the current IEEE-488 language in the FREQUENCY display field. If the display reads anything but L6080, press [0] to select the default language.

The language setting is stored in non-volatile memory and is retained when the power is turned off.

Section 5A
Remote Programming

INTRODUCTION 5A-1.

Communication between the controller and the Signal Generator consists of interface messages and commands. Interface messages are defined by the IEEE-488.1 standard and control the lowest level of bus communication. Interface messages are handled automatically by the controller. (The interface messages that the Signal Generator accepts and sends are listed in Tables 5A-4 and 5A-5.) Commands are sent to the Signal Generator literally, for example, with the Fluke 1722A BASIC PRINT statement. The commands are described in Tables 5B-1 and 5B-3. There are three types of commands:

1. Common commands

   Commands that start with an asterisk which are defined by the IEEE-488.2 standard.

2. Device-dependent commands

   Commands specific to the Signal Generator

3. Queries

   Commands that cause the Signal Generator to send a response to the controller. (These commands always end with a question mark (?).

A controller program first needs to initialize the interface and the Signal Generator. The following sample program can be used.

```
10 INIT PORT 0 \ REMOTE @2          ! PUT SIGNAL GENERATOR IN REMOTE
20 CLEAR @2                         ! CLEAR IEEE-488 INTERFACE
25 PRINT @2, "GAL"                  ! SET TO 488.2 LANGUAGE
30 PRINT @2, "*CLS; *RST"           ! CLEAR ERRORS & RESET SIG GEN
40 PRINT @2, "*SRE 0"               ! DON'T GENERATE SRQs
```

If the programmer wishes to use SRQs, the *SRE, *ESE, and ISCE commands should be used to enable the desired event. Refer to "Checking the Instrument Status" later in Section 5A for more information.

Programming the Signal Generator involves sending the desired commands to the instrument as shown in the following program.

```
100 PRINT @2, "FREQ 100 MHZ; AMPL -15 DBM" ! PROGRAM FREQUENCY AND AMPLITUDE
110 PRINT @2, "RFOUT ON"                   ! TURN RF OUTPUT ON
120 PRINT @2, "FM 1.2 KHZ; EXTAC_FM ON"    ! PROGRAM DEVIATION & ENABLE EXTERNAL FM
```

Instrument parameters can be retrieved with a query (programming commands that contain a question mark):

```
200 PRINT @2, "FREQ?"                ! RETRIEVE FREQUENCY
210 INPUT LINE @2, A$
220 PRINT "Frequency is: "; A$
230 PRINT @2, "RFOUT?"               ! RETRIEVE RF OUTPUT STATE
240 INPUT LINE @2, A$
250 PRINT "RF output is: "; A$
260 PRINT @2, "FM?; EXTAC_FM?"       ! RETRIEVE DEVIATION & EXTERNAL FM STATE
270 INPUT LINE @2, A$
280 PRINT "FM info is: "; A$
```

After the program has run, the output is:

```
Frequency is 1.000000000E+08,HZ
RF output is ON
FM info is 1.200E+03,HZ;ON
```

Programming errors may be checked by the following sample programs. The Error Available (EAV) bit in the serial poll register may be checked using a serial poll.

```
300 A = SPL(2)                              ! CHECK FOR ERRORS
310 IF (A AND 8) THEN PRINT "There was an error"
320 PRINT @2, "*CLS"                        ! CLEAR ERRORS
```

The error and an explanation can be checked as follows. Since errors are accumulated in a queue, the entire queue must be read to retrieve and clear all the errors.

```
400 PRINT @2, "ERROR? EXPLAIN"              ! CHECK FOR ERRORS
410 INPUT @2, A, A$
420 IF (A = 0) THEN GOTO 500                ! NO MORE ERRORS
430 PRINT "Error# :";A, A$                  ! PRINT ERROR# AND EXPLANATION
440 GOTO 400
500 END
```

COMMAND SYNTAX INFORMATION 5A-2.

The following syntax rules apply to all the remote commands. (A command consists of a word by itself or a word followed by one or more parameters.) The rules for parameter syntax are provided first (including proper usage of units), followed by the rules for extra spaces, followed by the rules for terminator usage. A description of how the Signal Generator processes incoming characters provides the basis for answering other possible questions about syntax. Information about syntax of response messages is also given.

Parameter Syntax Rules 5A-3.

Many of the remote commands require parameters. Improper use of parameters causes command errors to occur.

General rules for parameter usage are as follows:

1. When a command has more than one parameter, the parameters must be separated by commas.

   For example: "MEM_DIVIDER 1, 25, 30, 48".

2. Numeric parameters may have up to 255 significant digits and their exponents may range from -32000 to +32000. The useful range for Signal Generator programming is ± 2.2 E-308 to ± 1.8 E308.

3. Specifying more parameters than allowed by a particular command causes a command error.

4. Null parameters cause a command error (e.g., the adjacent commas in "MEM_DIVIDER 1, 25, , 48").

5. Expressions, for example "(4+2*13)", are not allowed as parameters.

Units that are accepted in command parameters are listed in Table 5B-1.

Extra Space Characters 5A-4.

Table 5B-3 and the remote program examples in this section show commands and their parameters separated by spaces. One space after a command is required. All other spaces are optional. They are shown for clarity in the manual and may be left in or omitted as desired. Extra spaces can be inserted between parameters as desired. Extra spaces within a parameter are generally not allowed, except for between a number and its associated unit.

EXAMPLE	EXPLANATION
FREQ 100 MHZ	Equivalent to "FREQ 100MHZ'
MEM_DIVIDER 1, 25, 30, 48	Equivalent to "MEM_DIVIDER 1,25,30,48"
AMPL -1 2.5 DBM	Invalid; no space allowed in a number
AMPL -12.5 DBM	Correct form for above

Table 5B-3 contains examples for commands whose parameters are not self explanatory. Remote program examples for the Fluke 1722A Instrument Controller are provided at the end of this section.

Terminators 5A-5.

To signify the end of a response sent to the controller, the Signal Generator sends a "terminator." The Signal Generator sends the ASCII character Line Feed (LF) with the EOI control line asserted as the terminator for response messages. The Signal Generator recognizes the following as terminators when encountered in incoming data:

- The ASCII LF character
- Any ASCII character sent with the EOI control line asserted

The terminator used by the Fluke 1722A Instrument Controller for data it sends to instruments on the IEEE-488 bus is programmable, but its default is LF with EOI.

Incoming Character Processing 5A-6.

The Signal Generator processes all incoming data as follows:

1. All data is taken as 7-bit ASCII, the eighth bit (DIO8) is ignored (except the 8-bit data byte portion of the *PUD and *DDT parameters).

2. Lower-case or upper-case characters are accepted.

3. ASCII characters whose decimal equivalent is less than 32 (Space) are discarded, except for characters 10 (LF) and 13 (CR) and in the *PUD and *DDT command arguments. The *PUD and *DDT commands allow all characters in their arguments, and they terminate in a special way.

Response Message Syntax 5A-7.

In Table 5B-3, responses from the Signal Generator are described wherever appropriate. In order to know whether to read an integer or a floating-point number, the entry is labeled "(Integer)" or "(Floating)".

Integers for most controllers or computers are decimal numbers in the range -32768 to 32767. Response elements of this type are labeled as "Integer" in the command tables. Floating-point numbers may be in exponential form, i.e., "1.15E-12". Examples in Table 5B-3 show response formats.

INPUT BUFFER OPERATION 5A-8.

As the Signal Generator receives each data byte from the controller, it places the bytes in a portion of memory called the input buffer. The input buffer holds up to 64 data bytes and operates in a first-in/first-out fashion.

The Signal Generator treats the IEEE-488 EOI control line as a separate data byte and inserts it into the input buffer if it is encountered as part of a message terminator.

The Signal Generator treats the IEEE-488 trigger interface message as a separate byte and inserts it into the input buffer at the time it is received.

Input buffer operation is transparent to the program running on the controller. If the controller sends commands faster than the Signal Generator can process them, the input buffer fills to capacity. When the input buffer is full, the Signal Generator holds off the IEEE-488 bus with the handshake lines. When the Signal Generator has processed a data byte from the full input buffer, it then completes the handshake, allowing the controller to send another data byte.

The Signal Generator clears the input buffer at power-on and on receiving the DCL (Device Clear) or SDC (Selected Device Clear) messages from the controller.

COMMANDS 5A-9.

Table 5B-1 summarizes the commands by function. Table 5B-3 provides protocol details of the remote commands. The commands duplicate almost all activities that can be initiated from the front panel in local operation. Separate headings for each command in the tables provide the parameters and responses (if any), and an example for cases in which the parameters are not self explanatory.

Multiple Commands 5A-10.

If the controller on the IEEE-488 bus is a Fluke 1722A, commands are sent one at a time, or combined, in Fluke BASIC PRINT statements. For example if the Signal Generator bus address is 2, use the following BASIC program statements to set the Signal Generator to output 100 MHz and -25 dBm.

```
10 INIT PORT 0 \ REMOTE @2  ! PUT SIGNAL GENERATOR IN THE REMOTE STATE
20 PRINT @2,"FREQ 100 MHZ"  ! PROGRAM 100 MHZ
30 PRINT @2,"AMPL -25 DBM"  ! PROGRAM -25 DBM
40 PRINT @2,"RFOUT ON"      ! TURN THE RF OUTPUT ON
```

The same results can be achieved by combining the three commands in one statement as follows (note that each command is separated by a ";"):

```
10 INIT PORT 0 \ REMOTE @2
20 PRINT @2,"FREQ 100 MHZ ; AMPL -25 DBM ; RFOUT ON"
```

Command Processing 5A-11.

All commands are processed in the order they are received. Each command is completely processed before the next is processed.

Table 5B-3 lists all the commands processed by the Signal Generator. Commands are received and executed at all times. Some restrictions may apply in certain Signal Generator modes of operation.

Command Restrictions 5A-12.

During sweep operation, some commands are rejected and some are processed differently. This information is noted in Table 5B-3 with the description of the commands.

In local, all calibration and compensation commands are rejected. (CAL_AM, CAL_FM, CAL_LEVEL, CAL_REFOSC, CMEM_FIX, COMP_ATT, COMP_COARSE, COMP_OUT, COMP_OUTDEF, COMP_SUBSYN, COMP_SUM)

During calibration and compensation procedures, only a subset of commands are allowed. Refer to the section "Closed-Case Calibration Adjustments" and the section "Compensation Procedures" in the Service Manual for details.

In listen-only, all calibration and compensation commands and all the queries (those that end with a "?") are rejected.

Commands That Require the CAL|COMP Switch To Be Set 5A-13.

CAUTION

Great care should be exercised in using these commands, as they may alter the Signal Generator calibration/compensation data.

The following commands do not work unless the rear panel CAL|COMP switch is in the 1 (on) position: *PUD, CMEM_FIX, and all commands that start with CAL_, CC_, and COMP_. Attempting to use any of these commands with the CAL|COMP switch in the 0 (off) position causes the Signal Generator to log an error into the error queue.

REMOTE/LOCAL STATE TRANSITIONS 5A-14.

The Signal Generator can be operated using the front panel keys as described in Section 4, "Front Panel Operation", or remotely using a remote controller. In addition, the Signal Generator can be placed in a local lockout condition at any time by command of the controller. When combined, the local, remote, and lockout conditions yield four possible operating states:

- Local

  The Signal Generator responds to local (front panel) and remote commands. This is also called "front panel operation." Some remote commands are not allowed in the local state. These are mostly procedural commands such as the calibration and compensation commands.

- Local with Lockout

  Local with lockout is identical to local, except the Signal Generator will go into the remote with lockout state instead of the remote state when it receives a remote command. The local with lockout state is entered by executing the Fluke 1722A BASIC "LOCKOUT" statement when using the 1722A as an IEEE-488 controller.

- Remote

  When the Remote Enable (REN) line is asserted and a controller addresses the Signal Generator as a listener, it enters the remote state. These conditions are met, for example, when a Fluke 1722A executes the BASIC statement "REMOTE \ PRINT @2'FREQ 100 MHZ'" if the Signal Generator's address is 2. In the remote state, the REMOTE annunciator is lit.

  Front panel operation is restricted to use of the power switch and the CLR|LCL key. Pressing this key returns the Signal Generator to the local state. The controller may also send a Go To Local (GTL) interface message. (When the Fluke 1722A is used, the "LOCAL @2" BASIC statement does this if the Signal Generator's address is 2.)

- Remote with Lockout

  The remote with lockout state can be entered from the remote state or from the local with lockout state, but not directly from the local state. Remote with lockout is similar to the remote state, but it is restricted: the CLR|LCL key does not return the Signal Generator to the local state. Instead, the message "Loc out" is displayed in the FREQUENCY display field when the key is pressed.

  To return the Signal Generator to the local with lockout state, the controller sends the Go To Local interface message (GTL). (When the Fluke 1722A is used as an IEEE-488 controller, the "LOCAL @2" BASIC statement does this if the Signal Generator's address is 2.)

Table 5A-1 summarizes the possible Remote/Local state transitions.

Table 5A-1. Remote/Local State Transitions

FROM	TO	USE	FLUKE 1722A BASIC COMMAND
Local	Remote	MLA + REN	REMOTE
	Local/Lockout	LLO + REN	LOCKOUT
Remote	Local	GTL, or CLR/LCL key	LOCAL
	Remote/Lockout	LLO + REN	LOCKOUT
Local/Lockout	Remote/Lockout	MLA + REN	REMOTE, or any Signal Generator command
Remote/Lockout	Local	$\overline{\text{REN}}$	LOCAL
	Local/Lockout	GTL	LOCAL @

CHECKING THE INSTRUMENT STATUS 5A-15.

The programmer has access to status registers, enable registers, and queues in the Signal Generator to indicate various conditions in the Signal Generator as shown in Figure 5A-1. Some of the registers and queues are defined by the IEEE-488.2 standard. The rest are specific to the Signal Generator.

Each status register and queue has a summary bit in the Serial Poll Status Byte. Enable registers are used to mask various bits in the status registers and generate summary bits in the Serial Poll Status Byte. The Service Request Enable Register can be used to assert the IEEE-488 Service Request (SRQ) control line on any one of the status conditions in the instrument.

Queries cause the Signal Generator response to be placed in the output queue. The output queue may contain responses from more than one query. The responses are output on a first-in/first-out basis, one at a time, in response to a controller input program statement. If the output queue is empty, no response will be sent to the controller.

Serial Poll Status Byte (STB) 5A-16.

The most important and frequently used register is the serial poll status byte, which the Signal Generator sends when it responds to a serial poll. The status byte can also be retrieved with the *STB? command. The value of this byte at power-on is determined by the value of the service request enable register (SRE), which is saved in non-volatile memory.

BIT ASSIGNMENTS FOR THE STB AND SRE 5A-17.

The bits in the Serial Poll Status Byte (STB) and Service Request Enable Register (SRE) are assigned as shown in Figure 5A-2.

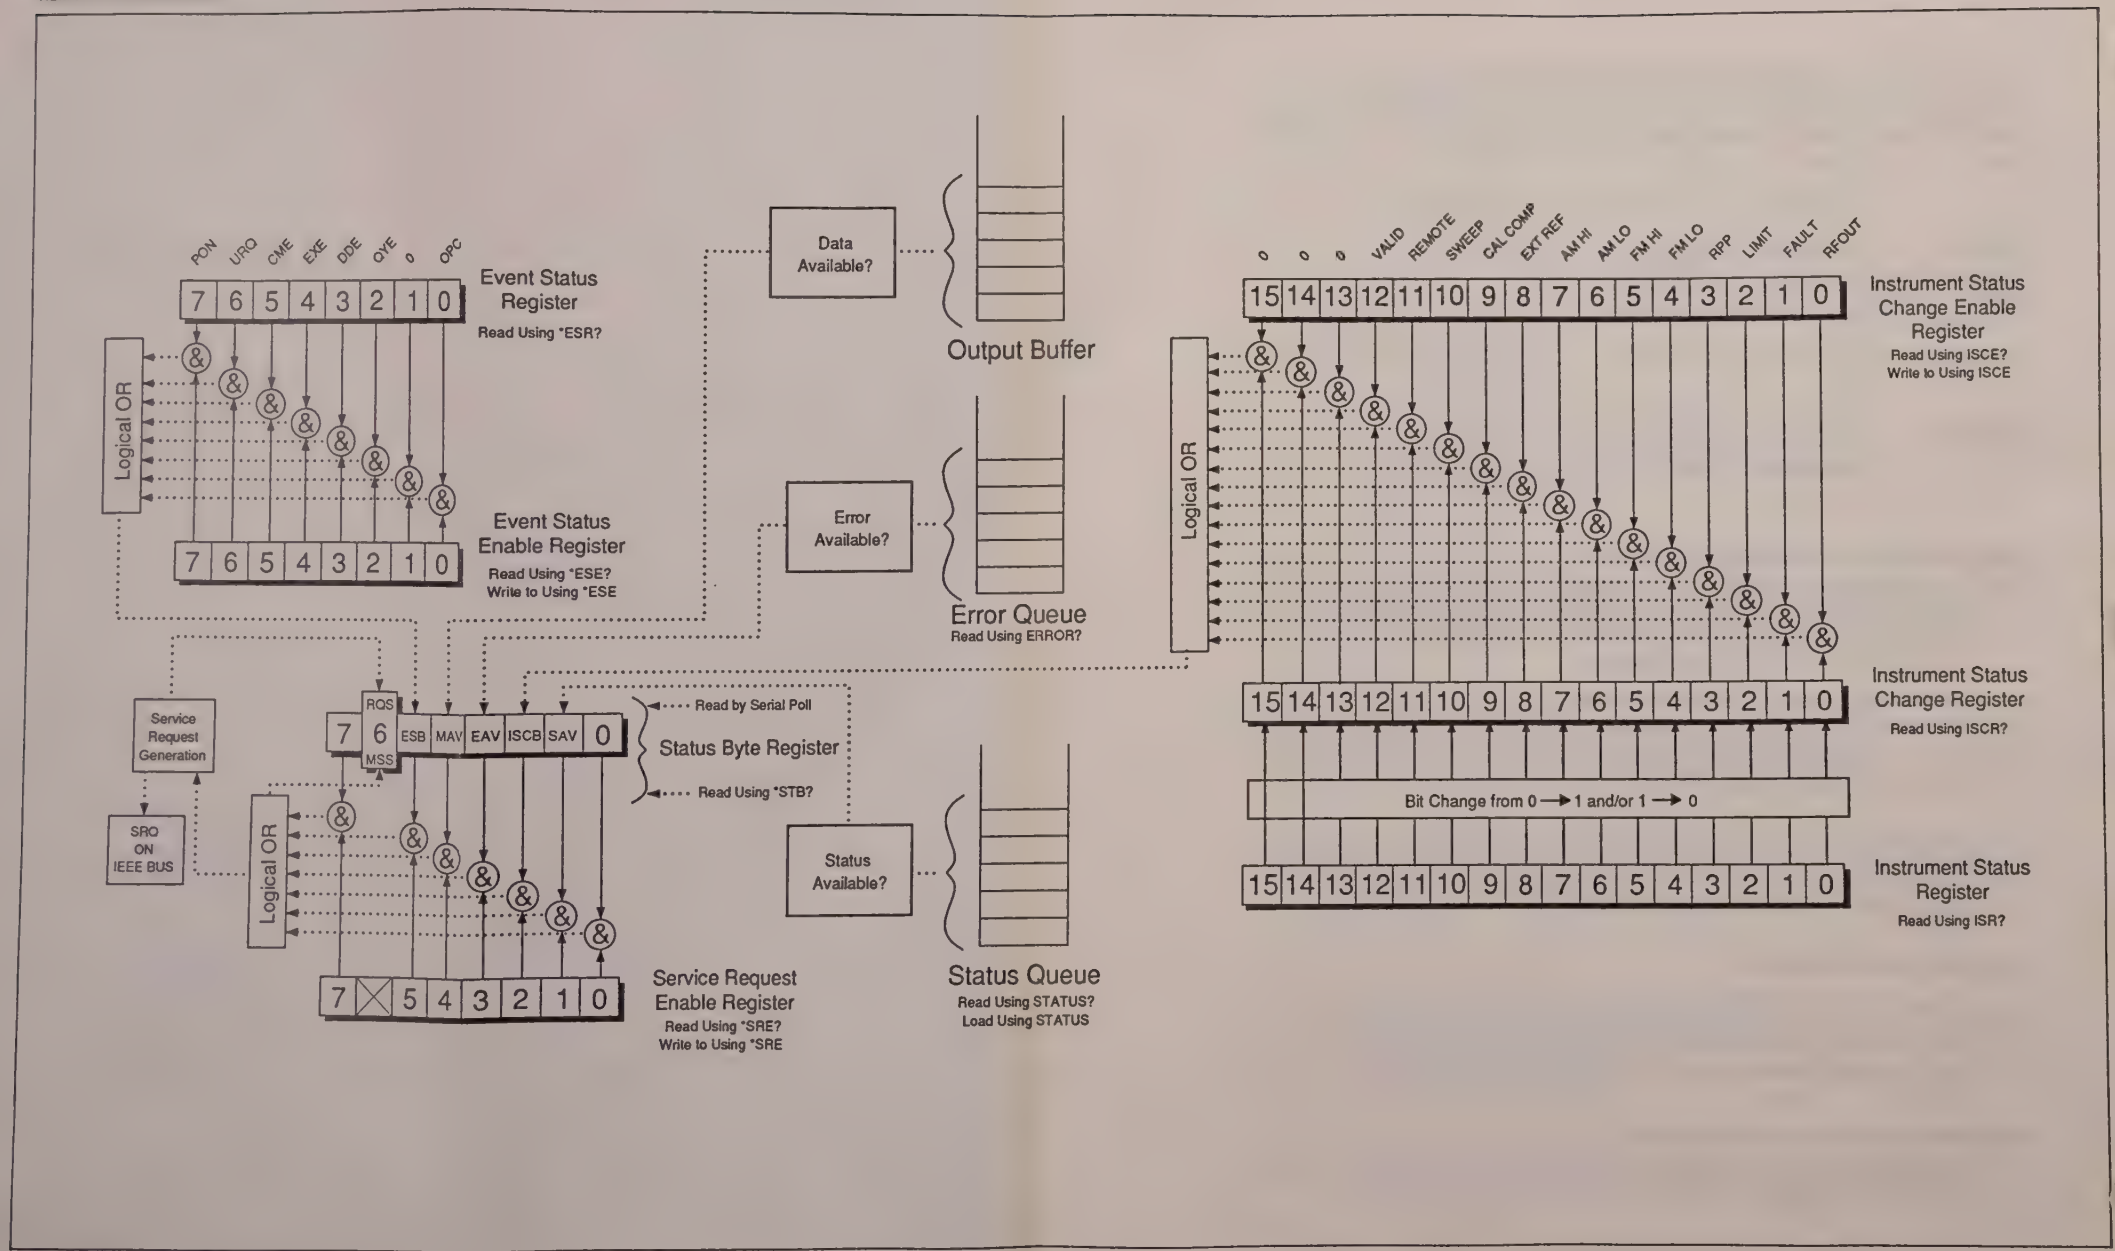
PON URQ CME EXE DDE QYE 0 OPC
7 6 5 4 3 2 1 0
Event Status Register
Read Using *ESR?
Logical OR
Event Status Enable Register
Read Using *ESE?
Write to Using *ESE
Data Available?
Output Buffer
Error Available?
Error Queue
Read Using ERROR?
0 0 0 VALID REMOTE SWEEP CAL COMP EXT REF AM HI AM LO FM HI FM LO RPP LIMIT FAULT RFOUT
15 14 13 12 11 10 9 8 7 6 5 4 3 2 1 0
Instrument Status Change Enable Register
Read Using ISCE?
Write to Using ISCE
Logical OR
Instrument Status Change Register
Read Using ISCR?
Bit Change from 0 → 1 and/or 1 → 0
Instrument Status Register
Read Using ISR?
Service Request Generation
SRQ ON IEEE BUS
RQS
MSS
ESB MAV EAV ISCB SAV
Read by Serial Poll
Status Byte Register
Read Using *STB?
Logical OR
Status Available?
Status Queue
Read Using STATUS?
Load Using STATUS
Service Request Enable Register
Read Using *SRE?
Write to Using *SRE

Figure 5A-1. Instrument Status Overview

7	6	5	4	3	2	1	0
0	RQS	ESB	MAV	EAV	ISCB	SAV	0
	MSS						

RQS Requesting service. The RQS bit is set to 1 whenever bits ESB, MAV, EAV, ISCB, or SAV change from 0 to 1 and are enabled (1) in the SRE. When RQS is 1, the Signal Generator asserts the SRQ control line on the IEEE-488 interface. You can do a serial poll to read this bit to see if the Signal Generator is the source of an SRQ.

MSS Master summary status. Set to 1 whenever bit ESB, MAV, EAV, ISCB, or SAV is 1 and enabled (1) in the SRE. This bit can be read using the *STB? command.

ESB Is set to 1 when one or more enabled ESR bits are 1.

MAV Message available. The MAV bit is set to 1 whenever data is available in the Signal Generator's IEEE-488 interface output buffer.

EAV Error available. An error has occurred and an error code is available to be read from the error queue using the ERROR? query.

ISCB One or more enabled ISCR bits are 1.

SAV Status available. Status codes have been loaded into the status queue and are available to be read from the queue using the STATUS? query.

Figure 5A-2. Bit Assignments for the STB and SRE

SERVICE REQUEST LINE (SRQ) 5A-18.

Service Request (SRQ) is an IEEE-488.1 bus control line that the Signal Generator asserts to notify the controller that it requires some type of service. Many instruments can be on the bus, but they all share a single SRQ line. To determine which instrument set SRQ, the controller normally does a serial poll of each instrument. The Signal Generator asserts SRQ whenever the RQS bit in its Serial Poll Status Byte is 1. This bit informs the controller that the Signal Generator was the source of the SRQ. The front panel SRQ annunciator is lit whenever the Signal Generator asserts SRQ.

The Signal Generator clears SRQ and RQS whenever the controller performs a serial poll of the Signal Generator IEEE-488 interface, sends *CLS, or whenever the MSS bit is cleared. The MSS bit is cleared only when ESB, MAV, EAV, ISCB, and SAV are 0, or when they are disabled by their associated enable bits in the SRE register being set to 0.

SERVICE REQUEST ENABLE REGISTER (SRE) 5A-19.

The Service Request Enable Register (SRE) enables or masks the bits of the Serial Poll Status Byte. The SRE is stored in non-volatile memory and is restored to its power-off value when the power is turned on.

PROGRAMMING THE STB AND SRE 5A-20.

The SRE can be set with the remote command *SRE and with a front panel special function sequence.

By setting the bits in the SRE, the associated bits in the Serial Poll Status Byte can be enabled. The following sample program enables the Error Available (EAV) bit.

```
10  ! THIS PROGRAM SETS EAV IN THE SRE
20  GOSUB 100                                  ! GET AND PRINT OLD SRE
30  IF ((A% AND 16%)=0%) THEN A% = A%+16%      ! ENABLE EAV (BIT 4)
40  PRINT @2,"*SRE ";A%                        ! "
50  GOSUB 100                                  ! GET AND PRINT NEW SRE
60  END
100 PRINT @2, "*SRE?"                          ! ASK FOR THE SRE CONTENTS
110 INPUT @2, A%                               ! RETRIEVE THE REGISTER CONTENTS
120 PRINT "SRE = ";A%
130 RETURN
```

The following front panel key sequence sets the SRE to be 16 (EAV enabled).

ENTER:	DISPLAY SHOWS:	EXPLANATION
SPCL 1 3	"SrE 12 ?"	Current value
0 1 6	"SrE 16 "	New value

The following program generates an error, and checks the Serial Poll Status Byte. Enable the EAV bit with the examples above.

```
10  ! THIS PROGRAM GENERATES AN ERROR AND CHECKS IT
20  PRINT @2, "FREQ 100 GHZ"                   ! CAN'T OUTPUT 100 GHZ
30  A% = SPL(2)                                ! DO A SERIAL POLL
40  IF ((A% AND 144%)=0%) THEN PRINT "EAV and SRQ should have been set"
50  PRINT @2, "STB?"                          ! RETRIEVE BYTE
60  INPUT @2, A%
70  IF ((A% AND 16%)=0%) THEN PRINT "EAV should have been set"
```

Event Status Register (ESR) 5A-21.

The Event Status Register is a two-byte register in which the higher eight bits are always 0, and the lower eight bits except bit 1 represent various conditions of the Signal Generator. The ESR is cleared (set to 0) when the power is turned on and every time it is read.

BIT ASSIGNMENTS FOR THE ESR AND ESE 5A-22.

The bits in the Event Status Register (ESR) and Event Status Enable Register (ESE) are assigned as shown in Figure 5A-3.

15	14	13	12	11	10	9	8
0	0	0	0	0	0	0	0

7	6	5	4	3	2	1	0
PON	URQ	CME	EXE	DDE	QYE	0	OPC

PON Power-on. This bit is set to 1 if the power supply has been turned off and on since the last time the ESR was read.

URQ User request. This bit is set on special function 14.

CME Command error. The Signal Generator's IEEE-488 interface encountered an incorrectly formed command. (The command ERROR? fetches the earliest error code in the error queue, which contains error codes for the first 15 errors that have occurred.)

EXE Execution error. An error occurred while the Signal Generator tried to execute the last command. This could be caused, for example, by a parameter being out of its allowed range or inconsistent with the generator's capabilities. An example would be attempting to execute "FREQ 100 GHZ", which is outside the range of the Signal Generator. (The command ERROR? fetches the earliest error in the error queue, which contains error codes for the first 15 errors that have occurred.)

DDE Device-dependent error. A error has occurred which is not a Command Error (CME), a Query Error (QYE), or an Execution Error (EXE). If a DDE occurs as the result of executing a command, it means that the command was formed properly and contained valid parameters, but some error condition arose during execution which prevented the command from completing properly. An example of a Device Dependent Error is error 90, "CAL|COMP switch not set to 1 (on)", which can occur when a calibration or compensation procedure is requested. (The command ERROR? fetches the earliest error in the error queue, which contains error codes for the first 15 errors that have occurred.)

QYE Query error. The Signal Generator was addressed to talk when no response data is present in the output queue and the instrument is not generating any response data via execution of a query. When a query error occurs, the Signal Generator clears the output queue, sets the QYE bit in the ESR register, and logs one of the four following error codes into the error queue according to the type of query error encountered:

Error 78: IEEE-488.2 UNTERMINATED Command

The unterminated command query error occurs when the controller attempts to read data from the Signal Generator's output queue without having first sent a valid query to the instrument. In this condition, the Signal Generator has nothing present in the output queue and is not in the process of generating a response to a query.Thus the instrument cannot respond to the controller's request for data.

Figure 5A-3. Bit Assignments for ESR and ESE

Error 79: IEEE-488.2 INTERRUPTED Query

Interrupted query occurs when the IEEE-488 controller sends a new character to the Signal Generator and response data is present in the output queue or the Signal Generator is generating response data by executing a query. After sending a query to the Signal Generator, the controller should always be sure to read all of the response data which the calibrator generates.

Error 80: IEEE-488.2 I/O DEADLOCK

This type of query error occurs when the Signal Generator has been asked to buffer more data than it has room to store in the output buffer. The Signal Generator logs this error when it detects the following three conditions simultaneously:

1. The output buffer is full, thus blocking completion the query which is generating response data.
2. The input buffer is full.
3. The controller is attempting to send a new character to the generator.

If these three conditions occur at the same time, the IEEE-488 bus will be blocked (deadlocked) since the controller cannot clear the condition unless it aborts sending the character and begins reading the output buffer.

OPC Operation complete. All commands previous to reception of a *OPC command have been executed, and the interface is ready to accept another message.

Figure 5A-3. Bit Assignments for ESR and ESE (cont)

EVENT STATUS ENABLE REGISTER (ESE) 5A-23.

A mask register called the Event Status Enable register (ESE) allows the controller to enable or mask (disable) each bit in the ESR. When a bit in the ESE is 1, the corresponding bit in the ESR is enabled. When any enabled bit in the ESR is 1, the ESB bit in the Serial Poll Status Byte also goes to 1. The ESR bit stays 1 until the controller reads the ESR or does a device clear, a selected device clear, or sends the clear status *CLS command to the Signal Generator. The ESE is stored in non-volatile memory and is restored when the power is turned on.

PROGRAMMING THE ESR AND ESE 5A-24.

To read the contents of the ESR, send the remote command, *ESR?. The ESR is cleared (set to 0) every time it is read. To read the contents of the ESE, send the remote command, *ESE?. The ESE is not cleared when it is read. When either register is read, the Signal Generator responds by sending a decimal number that represents bits 0 through 15.

The following sample program retrieves the contents of the ESR and ESE registers:

```
10  ! THIS PROGRAM READS THE ESR AND THE ESE REGISTERS
20  PRINT @2, "*ESR?"          ! ASK FOR THE ESR CONTENTS
30  INPUT @2, A%               ! RETRIEVE THE REGISTER CONTENTS
40  PRINT @2, "*ESE?"          ! ASK FOR THE ESE CONTENTS
50  INPUT @2, B%               ! RETRIEVE THE REGISTER CONTENTS
60  PRINT "ESR = ";A%          ! DISPLAY THE ESR REGISTER CONTENTS VALUE
70  PRINT "ESE = ";B%          ! DISPLAY THE ESE REGISTER CONTENTS VALUE
80  END
```

The status of the registers can be read by converting the contents of the variables A% and B% into binary. For example if A% is "32", its binary equivalent is: 00000000 00100000. Therefore, bit 5 (Command Error, CME) in the ESR is set (1) and the rest of the bits are reset (0). This means that the Signal Generator tried to execute an incorrectly formed command.

By setting the bits in the ESE, the associated bits in the ESR can be enabled. For example, to prevent the occurrence of a command error from causing bit 5 (ESB) in the Serial Poll Status Byte to go to 1, bit 5 in the ESE register can be reset (to 0).

The following sample program accomplishes this by checking the status of the CME bit, then toggling it if it is 1.

```
10  ! THIS PROGRAM RESETS BIT 5 (CME) IN THE ESE
20  PRINT @2,"*ESE 33"                  ! INITIAL ESE IS CME + OPC
30  GOSUB 100                           ! GET AND PRINT INITIAL ESE
40  IF (A% AND 32%) THEN A% = A% - 32% ! CLEAR CME (BIT 5)
50  PRINT @2, "*ESE ";A%                ! LOAD THE ESE WITH THE NEW VALUE
60  GOSUB 100                           ! GET AND PRINT NEW ESE
70  END
100 PRINT @2, "*ESE?"                   ! ASK FOR THE ESE CONTENTS
110 INPUT @2, A%                        ! RETRIEVE THE REGISTER CONTENTS
120 PRINT "ESE = ";A%
130 RETURN
```

The ESE may not be loaded from the front panel.

Output Queue 5A-25.

The output queue is loaded whenever a query is processed. The controller then reads it with a statement such as the Fluke 1722A BASIC INPUT statement. The Message Available (MAV) bit in the Serial Poll Status Byte indicates whether or not the output queue is empty.

If the queue is empty, the Signal Generator will not respond to the input statement from the controller.

The output queue is 64 characters long.

Error Queue 5A-26.

When a command error, execution error, query error, or device-dependent error occurs, its error code is placed in the error queue, where it can be read by the ERROR? command. All error codes are defined in Appendix C of this manual. ERROR? EXPLAIN will return the error code and a description of the error code.

Reading the first error with the ERROR? command removes that error from the queue. A response of "0" means the error queue is empty. The Error Available (EAV) bit in the Serial Poll Status Byte indicates whether or not the error queue is empty. The error queue is cleared when the Signal Generator is turned on and by the *CLS command.

The error queue contains up to 16 entries. If many errors occur, only the first 15 errors are kept in the queue. A 16th entry in the queue is always an "error queue overflow" error, and all later errors are discarded until the queue is at least partially read. Since many errors may occur before they are acknowledged and read, the earliest errors are the most likely to point to the problem. Subsequent errors are usually repetitions or consequences of the original problem.

Instrument Status Register (ISR) 5A-27.

The Instrument Status Register (ISR) gives the controller access to the state of the Signal Generator, including some of the information presented with the display annunciators on the front panel.

BIT ASSIGNMENTS FOR THE ISR, ISCR, AND ISCE 5A-28.

The bits in the Instrument Status Register (ISR), Instrument Status Change Register (ISCR), and Instrument Status Change Enable Register (ISCE) are assigned as shown in Figure 5A-4.

INSTRUMENT STATUS CHANGE REGISTER (ISCR) 5A-29.

The Instrument Status Change Register (ISCR) indicates which ISR bits have changed status (from 0 to 1 or from 1 to 0) since the ISCR was last read. The ISCR is cleared (set to 0) when the Signal Generator is turned on and every time it is read.

15	14	13	12	11	10	9	8
0	0	0	VALID	REMOTE	SWEEP	CALCOMP	EXTREF
			↑	↑↓	↓	↑↓	↑↓

7	6	5	4	3	2	1	0
AM HI	AM LO	FM HI	FM LO	RPP	LIMIT	FAULT	RFOUT
↑	↑	↑	↑	↑	↑	↑	↑↓

VALID When 1, the RF output is valid

REMOTE When 1, the Signal Generator is under remote control (REMOTE annunciator is lit).

SWEEP When 1, digital sweep is active.

CALCOMP When 1, the CAL|COMP switch is in the "1" position.

EXTREF When 1, the external reference frequency is being used (EXTREF switch is in the "EXT" position).

AM HI When 1, the external AM signal is greater than 1.02V.

AM LO When 1, the external AM signal is less than 0.98V.

FM HI When 1, the external FM signal is greater than 1.02V.

FM LO When 1, the external FM signal is less than .98V.

RPP When 1, the RPP circuitry has tripped.

LIMIT When 1, the Signal Generator is operating in a hardware limited region.

FAULT When 1, the Signal Generator has a hardware fault condition.

RFOUT When 1, the RF output is on.

Figure 5A-4. Bit Assignments for the ISR, ISCR, and ISCE

INSTRUMENT STATUS CHANGE ENABLE REGISTER 5A-30.

The Instrument Status Change Enable Register (ISCE) is a mask register for the ISCR. If a bit in the ISCE is enabled (set to 1) and the corresponding bit in the ISCR changes in the proper direction, the ISCB bit in the Serial Poll Status Byte is set to 1. ISCR bits marked ↑ set the change bit when the ISCR bit goes from a 0 to a 1, ISCR bits marked ↓ set the change bit when the ISCR bit goes from a 1 to a 0, and ISCR bits marked ↑ ↓ set the change bit when the ISCR bit changes. If all bits in the ISCE are disabled (set to 0), the ISCB bit in the Serial Poll Status Byte never goes to 1. The ISCE is stored in non-volatile memory and is restored to its power-off value when the power is turned on.

PROGRAMMING THE ISR, ISCR, AND ISCE 5A-31.

To read the contents of the ISR, send the remote command, ISR?. To read the contents of the ISCR, send the remote command, ISCR?. To read the contents of the ISCE, send the remote command, ISCE?. The Signal Generator responds by sending a decimal number that represents bits 0 through 15. Every time the ISCR is read, its contents are zeroed.

The following sample program reads the ISR, ISCR, and ISCE registers:

```
10  ! THIS PROGRAM READS THE ISR, ISCR, AND ISCE REGISTERS
20  ! NOTE THAT THE ICSR? COMMAND ALSO CLEARS THE ISCR CONTENTS
30  PRINT @2, "ISR?"      ! ASK THE ISR CONTENTS
40  INPUT @2,A%           ! RETRIEVE REGISTER CONTENTS FROM SIGNAL GENERATOR
50  PRINT @2, "ISCR?"     ! ASK FOR AND CLEAR THE ISCR CONTENTS
60  INPUT @2, B%          ! RETRIEVE REGISTER CONTENTS FROM SIGNAL GENERATOR
70  PRINT @2, "ISCE?"     ! ASK FOR THE ISCE CONTENTS
80  INPUT @2, C%          ! RETRIEVE REGISTER CONTENTS FROM SIGNAL GENERATOR
90  PRINT "ISR =  ";A%    ! DISPLAY THE ISR
100 PRINT "ISCR = ";B%    ! DISPLAY THE ISCR
110 PRINT "ISCE = ";C%    ! DISPLAY THE ISCE
120 END
```

The status of the instrument can be read by converting the returned variables into binary. For example, if a register contains "4", its binary equivalent is: 00000000 00000100. Therefore, bit 3 (CALCOMP) is set (1), and the rest of the bits are reset (0).

By setting the bits in the ISCE, the associated bits in the ISCR can be enabled. For example, to cause an SRQ interrupt when an the RPP trips, bit 3 (RPP) in the ISCE register must be 1. (The ISCB bit must also be enabled in the SRE.)

The following sample program loads a decimal 8 into the ISCE, which sets bit 3 and resets the other bits:

```
10  ! THIS PROGRAM LOADS 00000000 00001000 BINARY INTO THE ISCE
20  PRINT @2, "ISCE 8"     ! LOAD DECIMAL 8 INTO THE ISCE
30  PRINT @2, "ISCE?"      ! READ BACK THE VALUE
40  INPUT @2, A%           ! "
50  PRINT "ISCE = ";A%     ! PRINT IT, IT SHOULD BE 8
60  END
```

The ISCE cannot be loaded from the front panel.

Status Queue

5A-32.

The status queue is loaded with the STATUS command. The argument to the STATUS command (UNCAL, SELFTEST, CHECKSUM, or ORIGIN) indicates which status is to be loaded. The previous contents of the status queue are cleared when a new status is loaded with the STATUS command. Once the status queue is loaded, it can be read with successive STATUS? commands. A response of 0 indicates that the status queue is empty. All status codes are defined in Appendix D and E of this manual. STATUS? EXPLAIN will return the status code and a description of the status code.

Reading the first status with the STATUS? command removes that status from the queue. A response of "0" means the status queue is empty. The Status Available (SAV) bit in the Serial Poll Status Byte is "0" when the status queue is empty and "1" when the queue has been loaded with the STATUS command. The status queue is cleared when the Signal Generator is turned on and by the *CLS command.

IEEE-488 INTERFACE CONFIGURATION

5A-33.

The Signal Generator IEEE-488 interface supports the IEEE-488 interface function subsets listed in Table 5A-2.

Table 5A-2. IEEE-488 Interface Function Subsets Supported

INTERFACE FUNCTION	DESCRIPTION
SH1	Complete source handshake capability
AH1	Complete acceptor handshake capability
T5	Basic talker, serial poll, talk-only mode, Unaddress if MLA
TE0	No extended talker capability
L3	Basic listener operation, listen-only mode, Unaddress if MTA
LE0	No extended listener capabilities
SR1	Full service request capability, with bit-maskable SRQ
RL1	Full remote/local capability, including local lockout
PP0	No parallel poll capability
DC1	Device clear capability
DT1	Device trigger capability
C0	No bus control capability
E2	Tri-state drivers

BUS COMMUNICATION OVERVIEW

5A-34.

Communication between the controller and the Signal Generator takes place using commands established by IEEE-488 standards and commands specifically related to the Signal Generator. The commands in Tables 5B-1 and 5B-3 are all the remote commands, both common and device-dependent. Definitions of the different types of messages used on the IEEE-488 bus follow.

- Device-Dependent Commands

  Device-Dependent commands are messages used to transfer information directly between the Signal Generator and the IEEE-488 controller. Some commands cause an action to take place in the Signal Generator. Others, called queries in the

IEEE standards, ask for information, and always generate a response message from the instrument. While message format is governed by IEEE-488 standards, messages themselves are unique to the Signal Generator. For example, device-dependent commands are used to set the RF frequency and amplitude, and to turn the RF output on.

- Common Commands

  The IEEE standard 488.2 defines common commands, which are used for functions common to most bus devices. Examples include the command for resetting a device (*RST) and the query for device identification (*IDN?). Common commands and queries can be identified easily because they all begin with an asterisk (*).

- Interface Messages

  The IEEE standards define interface messages, which manage the interface system. Some of the interface messages have their own control lines, and others are sent over the data lines by first asserting the control line ATN (Attention). The IEEE-488 hardware within the controller handles interface messages, not the user or application program. For example, when a programming command is sent to the Signal Generator, the controller automatically sends the interface message MLA (My Listen Address).

Definition: Queries and Commands 5A-35.

Messages directed to the Signal Generator fall naturally into two categories: commands and queries. Commands (both common commands and device-dependent commands) instruct the Signal Generator to do something or to set a value; no response is expected. Queries generally ask for information from the Signal Generator, and do not set a value or instruct the instrument to do something; a response is always expected. Some queries also require the Signal Generator to take action. For example, the *TST? query has the Signal Generator do a self test, then send the result to the controller. A query always ends with a question mark. A command never ends with a question mark. Table 5B-3 does not separate commands and queries; they are all called commands and are presented together in one alphabetical list.

All query responses are generated instantly on receipt of the query. In other words, queries generate their output when the Signal Generator executes the query rather than when the controller attempts to read the response. The Signal Generator simply generates the requested message and places it in the output queue. When the controller addresses the Signal Generator as a talker, the contents of the output queue are transmitted to the controller.

Some messages have both query and command forms (e.g., *PUD and *PUD?). In such cases, the command generally sets the value of a parameter, and the query generally returns the most recent value of the parameter. Some messages are queries only (e.g., *IDN?). Some messages are commands only (e.g., *RST).

Functional Elements of Commands 5A-36.

Table 5A-3 lists the functional elements of commands described by the IEEE-488.2 standard that are used by the Signal Generator. This table is for those who have a copy of the standard and want to use it to pursue additional information. The standard provides full definitions and syntax diagrams for each element.

Table 5A-3. Functional Elements of Commands

ELEMENT	FUNCTION
PROGRAM MESSAGE	A sequence of zero or more PROGRAM MESSAGE UNIT elements separated by PROGRAM MESSAGE UNIT SEPARATOR elements.
PROGRAM MESSAGE UNIT	A single command, programming data, or query received by the device.
COMMAND MESSAGE UNIT	A single command or programming data received by the device.
QUERY MESSAGE UNIT	A single query sent from the controller to the device.
PROGRAM DATA	Any of the six program data types.
PROGRAM MESSAGE UNIT SEPARATOR	Separates PROGRAM MESSAGE UNIT elements from one another in a PROGRAM MESSAGE.
PROGRAM HEADER SEPARATOR	Separates the header from any associated PROGRAM DATA.
PROGRAM DATA SEPARATOR	Separates sequential PROGRAM DATA elements that are related to the same header.
PROGRAM MESSAGE TERMINATOR	Terminates a PROGRAM MESSAGE.
COMMAND PROGRAM HEADER	Specifies a function or operation. Used with any associated PROGRAM DATA elements.
QUERY PROGRAM HEADER	Similar to a COMMAND PROGRAM HEADER except a query indicator (?) shows that a response is expected from the device.
CHARACTER PROGRAM DATA	A data type suitable for sending short mnemonic data, generally used where a numeric data type is not suitable.
DECIMAL NUMERIC PROGRAM DATA	A data type suitable for sending decimal integers of decimal fractions with or without exponents.
NON-DECIMAL NUMERIC PROGRAM DATA	A data type suitable for sending integer numeric representations in base 16, 8, or 2.
SUFFIX PROGRAM DATA	An optional field following DECIMAL NUMERIC PROGRAM DATA used to indicate associated multipliers and units.
STRING PROGRAM DATA	A data type suitable for sending 7-bit ASCII character strings where the content needs to be "hidden" (by delimiters).
ARBITRARY BLOCK PROGRAM DATA	A data type suitable for sending blocks of arbitrary 8-bit information. Blocks are limited in size to 1024 bytes.

Interface Messages 5A-37.

Interface messages manage traffic on the bus. Device addressing and clearing, data handshaking, and commands to place status bytes on the bus are all directed by interface messages. Some of the interface messages are communicated by state transitions of dedicated control lines. The rest of the interface messages are sent over the data lines with the ATN signal true. (All device-dependent and common commands are sent over the data lines with the ATN signal false.)

IEEE-488 standards define interface messages. Table 5A-4 lists the interface messages that the Signal Generator accepts. Table 5A-4 also shows the BASIC statement to execute on the 1722A Controller to generate the interface message. Table 5A-5 lists the interface messages that the Signal Generator sends. The mnemonics listed in the tables are not sent in BASIC PRINT statements as commands are; in this way they are different from device-dependent and common commands.

Interface messages are handled automatically in most cases. For example, handshake messages DAV, DAC, and RFD automatically occur under the direction of an instrument's interface itself as each byte is sent over the bus.

Table 5A-4. Interface Messages that the Signal Generator Accepts

MNEMONIC	NAME	FUNCTION	RELATED FLUKE 1722A BASIC COMMAND
ATN	Attention	A control line that, when asserted, notifies all instruments on the bus that the next data bytes are an interface message. When ATN is low, the next data bytes are interpreted as device-dependent or common commands addressed to a specific instrument.	(None)
DAC	Data Accepted	Sets the handshake signal line NDAC low.	(None)
DAV	Data Valid	Asserts the handshake signal line DAV.	(None)
DCL	Device Clear	Clears the input/output buffers.	CLEAR
END	End	A message that occurs when the Controller asserts the EOI signal line before sending a byte.	(None)
GET	Group Execute Trigger	Execute the command string predefined with the *DDT command.	TRIG @
GTL	Go To Local	Transfers control of the Signal Generator from one of the remote states to one of the local states. (See Table 5A-5.)	LOCAL @
LLO	Local Lockout	Transfers remote/local control of the Signal Generator. (See Table 5A-5.)	LOCKOUT

Table 5A-4. Interface Messages that the Signal Generator Accepts (cont)

MNEMONIC	NAME	FUNCTION	RELATED FLUKE 1722A BASIC COMMAND
IFC	Interface Clear	A control line that sets the interface to a quiescent state.	INIT
MLA	My Listen Address	Addresses a specific device on the bus as a listener. The controller sends MLA automatically whenever it directs a device-dependent or common command to a specific instrument.	(None)
MTA	My Talk Address	Addresses a specific device on the bus as a talker. The controller sends MTA automatically whenever it directs a device-dependent or common query to a specific instrument.	(None)
REN	Remote Enable	Transfers remote/local control of the Signal Generator. (See Table 5A-5.)	REMOTE
RFD	Ready for Data	Sets the handshake signal line NRFD low.	(None)
SDC	Selected Device Clear	Does the same thing as DCL, but only if the Signal Generator is currently addressed as a listener.	CLEAR @
SPD	Serial Poll Disable	Cancels the effect of a Serial Poll Enable.	(Part of SPL)
SPE	Serial Poll Enable	After the Signal Generator receives this message, it sends the Status Byte the next time it is addressed as a listener, no matter what the command is.	(Part of SPL)
UNL	Unlisten	"Unaddresses" a specific device on the bus as a listener. The controller sends UNL automatically after the device has successfully received a device-dependent or common command.	(None)
UNT	Untalk	"Unaddresses" a specific device on the bus as a listener. The controller sends UNT automatically after it receives the response from a device-dependent or common query.	(None)

Table 5A-5. Interface Messages that the Signal Generator Sends

MNEMONIC	NAME	FUNCTION
END	End	A message that occurs when the Signal Generator asserts the EOI control line. The Signal Generator asserts EOI while it transmits the ASCII character LF for its termination sequence or terminator.
DAC	Data Accepted	Sets the handshake signal line NDAC low.
DAV	Data Valid	Asserts the handshake signal line DAV.
RFD	Ready for Data	Sets the handshake signal line NRFD low.
SRQ	Service Request	A control line that any device on the bus can assert to indicate that it requires attention. Refer to "Checking Signal Generator Status" for details.
STB	Status Byte	The Status Byte is what the Signal Generator sends when it responds to a serial poll (interface message SPE).

THE IEEE-488 CONNECTOR 5A-38.

The IEEE-488 connector on the rear panel mates with an IEEE-488 Standard cable. The pin assignments of the rear-panel IEEE-488 connector are shown in Figure 5A-5.

The IEEE-488 Interface signal SHIELD (pin 12) can be disconnected (when using an IEEE-488 cable without a metallic hood) from the instrument ground. To do this, use the SHIELD switch.

The following restrictions apply to all IEEE-488 systems:

1. A maximum of 15 devices can be connected in a single IEEE-488 bus system.

2. The maximum length of IEEE-488 cable used in one IEEE-488 system is the lesser of either 20 meters or 2 meters times the number of devices in the system.

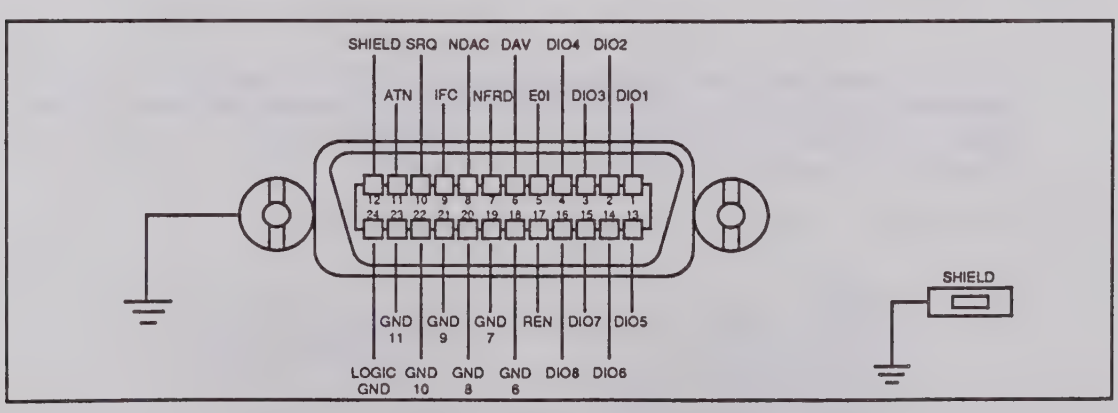

Figure 5A-5. IEEE-488 Connector Pinout (Rear Panel View)

REMOTE PROGRAM EXAMPLES 5A-39.

The following programs are written in BASIC for the Fluke 1722A Instrument Controller.

Using the *OPC?, *OPC, and *WAI Commands 5A-40.

The *OPC?, *OPC, and *WAI commands let the programmer maintain control of the order of execution of commands that could otherwise be passed up by subsequent commands.

If a FREQ command has been sent, the output can be checked to see if it has settled by sending the query *OPC?. As soon as the FREQ command has completed (output settled), a "1" appears in the output queue. The *OPC? command should always be followed with a read command (for example, in Fluke BASIC, "INPUT @2, A"). The read command causes program execution to pause until the addressed instrument responds.

The following sample program shows how *OPC? can be used.

```
10  PRINT @2, "FREQ 100MHZ;*OPC?"        ! SIGNAL GENERATOR ADDRESS IS 2
20  INPUT @2, A                           ! READ "1" FROM SIGNAL GENERATOR
30  !PROGRAM HALTS HERE UNTIL A "1" IS PUT INTO THE OUTPUT QUEUE
40  PRINT "OUTPUT SETTLED"
```

The *OPC command is similar in operation to the *OPC? query, except that it sets bit 0 (OPC for "Operation Complete") in the Event Status Register to 1 rather than sending a "1" to the output queue. One use for *OPC is to include it in a program so that it generates an SRQ (Service Request). Then an SRQ handler written into the program can detect the operation complete condition and respond appropriately. The *OPC command is similar to *OPC?, except the program must read the ESR to detect the completion of all operations.

The following sample program shows how *OPC can be used.

```
10  REMOTE
20  PRINT @2, "FREQ 100MHZ;*OPC"     ! SIGNAL GENERATOR ADDRESS IS 2
30  PRINT @2, "*ESR?"                ! PUT THE ESR BYTE IN BUFFER
40  INPUT @2, A%                     ! READ THE ESR BYTE
50  IF (A% AND 1%) = 0% GOTO 30      ! TRY AGAIN IF NO OPC
60  PRINT "OUTPUT SETTLED"
70  END
```

The *WAI command causes the Signal Generator to wait until any prior commands have been completed before continuing on to the next command, and takes no other action. Using *WAI is a convenient way to halt controller program execution until the command or commands preceding it have completed.

The following sample program shows how *WAI can be used.

```
10  REMOTE
20  PRINT @2, "FREQ 100MHZ;*WAI"     ! SIGNAL GENERATOR ADDRESS IS 2
30  PRINT @2, "FREQ?"                ! READ THE OUTPUT VALUE
40  INPUT @2, A$                     ! A$ CONTAINS THE OUTPUT VALUE
50  PRINT "OUTPUT SETTLED"
60  PRINT "OUTPUT IS: ";A$
70  END
```

Using the *DDT and *TRG Commands 5A-41.

The *DDT command is used to define the device trigger buffer. Once it is loaded, the stored commands may be executed with the *TRG command or the Group Execute Trigger (GET) interface message (Fluke 1722A BASIC TRIG command).

The use of the trigger buffer will speed up execution of the application program because the contents of the buffer do not need to be transferred on the IEEE-488 bus each time they are executed.

In the following example, the Signal Generator is programmed to step frequency approximately every second.

```
10  REMOTE
20  PRINT @2, "FREQ 210 MHZ"          ! SIGNAL GENERATOR ADDRESS IS 2
30  PRINT @2, "FREQ_STEP 1.25 KHZ"    ! PROGRAM STEP SIZE TO 1.25 KHZ
40  PRINT @2, "*DDT #0STEP_FREQ UP"   ! LOAD TRIGGER BUFFER
50  PRINT @2, "*DDT?"                 ! VERIFY CONTENTS OF BUFFER
60  INPUT LINE @2, A$ \ PRINT A$      ! A$ SHOULD BE "#213STEP_FREQ UP"
100 TRIG @2                           ! TRIGGER THE SIGNAL GENERATOR
110 WAIT 1000                         ! WAIT ~1 SECOND
120 GOTO 100                          ! DO IT AGAIN
```

Section 5B
Remote Command Tables

REMOTE COMMAND SUMMARY 5B-1.

Remote commands, organized by function, are summarized in Table 5B-1. Units that are accepted in command parameters are listed in Table 5B-2.

REMOTE COMMANDS 5B-2.

The complete list and description of remote commands, arranged in alphabetical order, is provided in Table 5B-3.

Table 5B-1. Remote Command Summary

RF FREQUENCY	
EXTREF_FREQ	Select the external reference frequency
EXTREF_FREQ?	Retrieve the selected external reference frequency
FREQ	Program the displayed rf output frequency
FREQ?	Retrieve the displayed rf output frequency
FREQ_ABS?	Retrieve the rf output frequency
FREQ_BASE?	Retrieve the base frequency
FREQ_REL	Select relative frequency mode
FREQ_REL?	Retrieve the state of relative frequency mode
REF?	Retrieve the setting of the frequency reference (INT/EXT)
RF OUTPUT AMPLITUDE	
AMPL	Program the displayed rf output amplitude
AMPL?	Retrieve the displayed rf output amplitude
AMPL_ABS?	Retrieve the rf output level
AMPL_BASE?	Retrieve the base amplitude
AMPL_CMPDAT	Select alternate output level compensation data
AMPL_CMPDAT?	Retrieve the alternate output level compensation state
AMPL_COMP	Select the amplitude compensation mode
AMPL_COMP?	Retrieve the state of amplitude compensation mode
AMPL_EMFOUT	Select EMF display mode
AMPL_EMFOUT?	Retrieve the state of EMF display mode
AMPL_RANGE	Select amplitude normal/fixed range mode
AMPL_RANGE?	Retrieve the state of amplitude range mode
AMPL_REL	Select relative amplitude mode
AMPL_REL?	Retrieve the state of relative amplitude mode
AMPL_UNITS	Convert the AMPLITUDE display to specified units
RFOUT	Turn the RF OUTPUT port ON or OFF
RFOUT?	Retrieve the state of the RF OUTPUT port
PHASE ADJUST	
PHASE	Adjust the phase of the rf carrier
PHASE?	Retrieve the relative phase adjustment
PHASE_CLK	Program the measured phase adjustment clock frequency
PHASE_CLK?	Retrieve the phase adjustment clock frequency
PHASE_ZERO	Zero the relative phase adjustment
AMPLITUDE MODULATION	
AM	Program the AM depth
AM?	Retrieve the AM depth
EXTAC_AM	Turns external ac-coupled AM ON or OFF
EXTAC_AM?	Retrieve the state of external ac-coupled AM
EXTDC_AM	Turn external dc-coupled AM ON or OFF
EXTDC_AM?	Retrieve the state of external dc-coupled AM
INT_AM	Turn internal AM ON or OFF
INT_AM?	Retrieve the state of internal AM

Table 5B-1. Remote Command Summary (cont)

FREQUENCY AND PHASE MODULATION	
EXTAC_FM	Turn external ac-coupled FM/ØM ON or OFF
EXTAC_FM?	Retrieve the state of external ac-coupled FM/ØM
EXTDC_FM	Turn external dc-coupled FM or ØM ON or OFF
EXTDC_FM?	Retrieve the state of external dc-coupled FM or ØM
FM	Program the FM/ØM deviation
FM?	Retrieve the FM/ØM deviation
FM_RANGE	Select normal, low-distortion, or fixed-range FM
FM_RANGE?	Retrieve the state of low distortion/fixed range FM
FM_UNITS	Convert the FM display to specified units
HIRATEPM	Turn high rate ØM mode ON or OFF
HIRATEPM?	Retrieve the state of high rate ØM mode
INT_FM	Turn internal FM/ØM ON or OFF
INT_FM?	Retrieve the state of internal FM/ØM
LORATEFM	Turn low rate FM mode ON or OFF
LORATEFM?	Retrieve the state of low rate FM mode
PULSE MODULATION	
EXT_PULSE	Turn external pulse modulation ON or OFF
EXT_PULSE?	Retrieve the state of external pulse modulation
INT_PULSE	Turn internal pulse modulation ON or OFF
INT_PULSE?	Retrieve the state of internal pulse modulation
INTERNAL MODULATION OSCILLATOR	
MOD_WAVE	Select the modulation oscillator waveform
MOD_WAVE?	Retrieve the modulation oscillator waveform
MODF	Program the modulation frequency
MODF?	Retrieve the modulation frequency
MODL	Program the modulation level
MODL?	Retrieve the modulation level
MODOUT	Select the state of the MOD OUTPUT port
MODOUT?	Retrieve the state of the MOD OUTPUT port
PULSE_WIDTH	Program the modulation oscillator pulse width
PULSE_WIDTH?	Retrieve the modulation oscillator pulse width
SWEEP	
AMPL_MANUAL	Increment or decrements manual amplitude sweep
AMPL_SINCR	Program the amplitude sweep increment
AMPL_SINCR?	Retrieve the amplitude sweep increment
AMPL_SWIDTH	Program the amplitude sweep width
AMPL_SWIDTH?	Retrieve the amplitude sweep width
FREQ_MANUAL	Increment or decrement the manual frequency sweep
FREQ_SINCR	Program the frequency sweep increment
FREQ_SINCR?	Retrieve the frequency sweep increment
FREQ_SWIDTH	Program the frequency sweep width

Table 5B-1. Remote Command Summary (cont)

FREQ_SWIDTH?	Retrieve the frequency sweep width
SWEEP	Select the sweep mode
SWEEP?	Retrieve the sweep mode
SWEEP_DWELL	Program the sweep dwell time
SWEEP_DWELL?	Retrieve the sweep dwell time
SWEEP_FIELD	Select the sweep field
SWEEP_FIELD?	Retrieve the sweep field
SWEEP_SYM	Select the sweep symmetry
SWEEP_SYM?	Retrieve the sweep symmetry
MISCELLANEOUS	
*DDT	Define the device trigger buffer
*DDT?	Query the device trigger buffer
DISPLAY	Select the display status
DISPLAY?	Retrieve the display status
GAL	Go to alternate language
KEY_RATE	Select the repeat rate for the step keys
KEY_RATE?	Retrieve the key repeat rate
KNOB_STEP	Select the operation of the knob and step up/down keys
KNOB_STEP?	Retrieve the state of the knob and step up/down keys
LOCALERT	Program mode to generate an SRQ on complete front panel operations
LOCALERT?	Retrieve the state of the local alert (LOCALERT) mode
MOD_DISPLAY	Select the quantity to be shown in the modulation field
MOD_DISPLAY?	Retrieve the quantity shown in the modulation field
*OPC	Program bit 0 in the ESR when pending remote operations are completes
*OPC?	Replies with "1" when all pending operations are complete
*OPT?	Retrieve report of installed options
PRESET	Reset instrument to preset state
*PUD	Define protected user data buffer
*PUD?	Retrieve protected user data buffer
SPCL	Select a special function by number
*RST	Reset instrument to default memory location
*TRG	Trigger device
*WAI	Wait until all pending remote operations are complete
INSTRUMENT STATE MEMORY	
MEM_DIVIDER	Program memory divider locations
MEM_DIVIDER?	Retrieve memory divider locations
MEM_LOCK	Write-protects instrument state memory
MEM_LOCK?	Retrieve the state of memory lock protection
MEM_RESET	Reset all memory locations to instrument default
*RCL	Recall a memory location
*SAV	Save to a memory location
SEQ	Recall the next or previous memory location

Table 5B-1. Remote Command Summary (cont)

STEP	
AM_STEP	Program the AM depth step size
AM_STEP?	Retrieve the AM depth step size
AMPL_STEP	Program the rf output amplitude step size
AMPL_STEP?	Retrieve the rf output amplitude step size
FM_STEP	Program the FM/ØM deviation step size
FM_STEP?	Retrieve the FM/ØM deviation step size
FREQ_STEP	Program the output frequency step size
FREQ_STEP?	Retrieve the output frequency step size
MODF_STEP	Program the modulation frequency step size
MODF_STEP?	Retrieve the modulation frequency step size
MODL_STEP	Program the modulation level step size
MODL_STEP?	Retrieve the modulation level step size
SD	Step the active step field down by one step size
STEP_AM	Step the AM depth up or down by one step size
STEP_AMPL	Step the output amplitude up or down by one step size
STEP_FIELD	Select the step field
STEP_FIELD?	Retrieve the step field
STEP_FM	Step the FM/ØM deviation up or down by one step size
STEP_FREQ	Step the output frequency up or down by one step size
STEP_MODF	Step the modulation frequency up or down by one step size
STEP_MODL	Step the modulation level up or down by one step size
SU	Step the active step field up by one step size
EDIT	
AM_BRT	Move bright digit to specified decade in AM field
AM_BRT?	Retrieve decade of AM bright-digit position
AMPL_BRT	Move bright digit to specified decade in amplitude field
AMPL_BRT?	Retrieve decade of amplitude bright-digit position
BRT_FIELD	Program bright-digit field
BRT_FIELD?	Retrieve current bright-digit field
EDIT_AM	Select AM bright-digit field and edits AM
EDIT_AMPL	Select amplitude bright-digit field and edits amplitude
EDIT_FM	Select FM/ØM bright-digit field and edits FM/ØM
EDIT_FREQ	Select frequency bright-digit field and edits frequency
EDIT_MODF	Select modulation freq bright-digit field and edits modulation freq
EDIT_MODL	Select modulation level bright-digit field and edits modulation level
FM_BRT	Move bright digit to specified decade in FM/ØM field
FM_BRT?	Retrieve decade of FM/ØM bright-digit position
FREQ_BRT	Move bright digit to specified decade in frequency field
FREQ_BRT?	Retrieve decade of frequency bright-digit position
MODF_BRT	Move bright digit to specified decade in modulation freq field
MODF_BRT?	Retrieve decade of modulation frequency bright-digit position
MODL_BRT	Move bright digit to specified decade in modulation level field
MODL_BRT?	Retrieve decade of modulation level bright-digit position

Table 5B-1. Remote Command Summary (cont)

STATUS/ERROR	
*CLS	Clear status
ERROR?	Retrieve an error code from the error queue
*ESE	Load Event Status Enable register
*ESE?	Retrieve Event Status Enable register
*ESR?	Retrieve and clear the Event Status Register
EXPLAIN?	Explain a status/error code
*IDN?	Retrieve instrument identification.
ISCE	Load Instrument Status Change Enable register
ISCE?	Retrieve Instrument Status Change Enable register
ISCR?	Retrieve and clear Instrument Status Change Register
ISR?	Retrieve and clear Instrument Status Register
*SRE	Load Service Request Enable register
*SRE?	Retrieve Service Request Enable register
STATUS	Load specified status into the status queue
STATUS?	Retrieve a status code from the status queue
*STB?	Retrieve the status byte
SERVICE	
ATT_LOG?	Retrieve the attenuator log
CAL_AM	Initiate AM calibration procedure
CAL_FM	Initiate FM calibration procedure
CAL_LEVEL	Initiate level calibration procedure
CAL_REFOSC	Initiate reference oscillator calibration procedure
CC_ERRFREQ?	Returns frequency where automatic compensation procedure failed
CC_EXIT	Exit calibration/compensation procedure
CC_FREQ?	Retrieve the rf output frequency during calibration/compensation procedure
CC_RDAM	Report measured AM depth to calibration procedure
CC_RDDVM	Report measured voltage to compensation procedure
CC_RDFM	Report measured FM deviation to calibration procedure
CC_RDFREQ	Report measured rf output frequency to calibration procedure
CC_RDPOWER	Report measured power to cal/comp procedure
CC_SAVE	Calculate corrections, save new data in cal/comp memory
CC_TARGET?	Return target value of compensation procedure
CMEM_FIX	Repair compensation memory checksum errors
COMP_ATT	Initiate attenuator compensation procedure
COMP_COARSE	Initiate automatic coarse loop compensation procedure
COMP_OUT	Initiate output compensation procedure
COMP_OUTDEF	Initiate output compensation procedure with default
COMP_SUBSYN	Initiate subsynthesizer compensation procedure
COMP_SUM	Initiate automatic sum loop compensation procedure
ETIME?	Retrieve the elapsed time
TEST_ATT	Program alternate attenuator settings
TEST_DISP	Execute display test
*TST?	Execute self-test

Table 5B-2. Units Used with Remote Commands

UNIT	DESCRIPTION
HZ	Frequency, hertz
KHZ	Frequency, kilohertz
MHZ	Frequency, megahertz
MAHZ	Frequency, megahertz
GHZ	Frequency, gigahertz
V	Voltage (amplitude), volts
MV	Voltage (amplitude), millivolts
UV	Voltage (amplitude), microvolts
NV	Voltage (amplitude), nanovolts
DBMV	Voltage (amplitude), decibels referenced to 1 millivolt
DBUV	Voltage (amplitude), decibels referenced to 1 microvolt
DB	Ratio, decibels
DBM	Power (amplitude), decibels referenced to 1 milliwatt
DBMW	Power (amplitude), decibels referenced to 1 milliwatt
DBF	Power (amplitude), decibels referenced to 1 femtowatt
DBFW	Power (amplitude), decibels referenced to 1 femtowatt
PCT	Ratio (AM depth), percent
%	Ratio (AM depth), percent
RAD	Angle (ØM phase), radians
S	Time, seconds
MS	Time, milliseconds
US	Time, microseconds

Table 5B-3. Remote Commands

AM

Description:	Program the AM depth in percent. The default units are PCT.
Parameter:	AM depth with optional PCT or % units.
Examples:	AM 63.2 PCT AM 63.2 %
Restrictions:	Rejected during manual or single sweep.

AM?

Description:	Retrieve the AM depth.
Parameter:	None
Responses:	1. (Float) AM depth. 2. (String) PCT
Example:	6.320E+01,PCT

AM_BRT

Description:	Move the bright digit to specified decade in AM field. The default units are PCT.
Parameter:	Bright-digit decade in AM display with optional PCT or % units.
Examples:	AM_BRT 1 PCT AM_BRT 1 %
Restrictions:	Rejected during manual or single sweep.

AM_BRT?

Description:	Retrieve the decade of AM bright-digit position.
Parameter:	None
Response:	1. (Float) Bright-digit decade in AM display. 2. (String) PCT
Example:	1.0E+0,PCT

AM_STEP

Description:	Program the AM depth step size in percent. The default units are PCT.
Parameter:	AM depth step size with optional PCT or % units.
Restrictions:	Rejected during manual or single sweep.

AM_STEP?

Description:	Retrieve the AM depth step size.
Parameter:	None
Response:	1. (Float) AM depth step size. 2. (String) PCT

Table 5B-3. Remote Commands (cont)

AMPL

Description: Program the displayed RF amplitude in dBm, dBμV, dBmV, dBf, dB, or V. Default units are DBM. If REL_AMPL is OFF, this is the output RF level. Refer to Section 4B, "RF Amplitude" for more details. If Auto Amplitude Sweep is active, programs the center Amplitude. Refer to Section 4E, "Sweep" for more information.

Parameter: Displayed RF amplitude with optional power, voltage, or DB units.

Examples:
AMPL 174 MV
AMPL –10.0

Restrictions: Rejected during manual or single sweep.

AMPL?

Description: Retrieve the displayed RF amplitude. If REL_AMPL is OFF, this is the output RF level. If Amplitude Sweep is active, returns the center Amplitude. Refer to section 4E, "Sweep" for more information.

Parameter: None

Responses:
1. (Float) Displayed RF amplitude.
2. (String) DBM, DBUV, DBMV, DBF, DB, V, DBUV-EMF, DBMV-EMF, or V-EMF

Examples:
1.7400E-01,V
–1.0000E+01,DBM

AMPL_ABS?

Description: Retrieve the RF output level.

Parameter: None

Responses:
1. (Float) Output RF amplitude.
2. (String) DBM, DBUV, DBMV, DBF, V, DBUV-EMF, DBMV-EMF, or V-EMF

AMPL_BASE?

Description: Retrieve the base amplitude. If AMPL_REL is OFF, this value is 0 dB. Refer to Section 4B, "RF Amplitude" for more details.

Parameter: None

Responses:
1. (Float) Base RF amplitude.
2. (String) DB, V, or V-EMF

Table 5B-3. Remote Commands (cont)

AMPL_BRT

Description:	Move the bright digit to specified decade in amplitude field. Note that the units must match the displayed units (e.g. V, MV, UV or NV for Volts; DBM, DBUV, DBMV, or DBF for dB) when specifying the bright-digit position. The default units are DBM.
Parameter:	Bright-digit decade in AMPLITUDE display field with optional power, voltage, or DB units.
Examples:	AMPL_BRT 10 UV AMPL_BRT .1 DBM
Restrictions:	Rejected during manual or single sweep.

AMPL_BRT?

Description:	Retrieve the decade of amplitude bright-digit position.
Parameter:	None
Responses:	1. (Float) Bright-digit decade in AMPLITUDE display field. 2. (String) DBM, DBUV, DBMV, DB, or V
Example:	1.0E–7,V

AMPL_CMPDAT

Description:	Select standard or alternate output level compensation data.
Parameter:	STD or ALT
Restrictions:	Rejected during sweep.

AMPL_CMPDAT?

Description:	Retrieve the output level compensation state.
Response:	(String) STD or ALT

AMPL_COMP

Description:	Select the amplitude compensation mode.
Parameter:	ALL or OUTPUT or NONE
Restrictions:	Rejected during sweep.

AMPL_COMP?

Description:	Retrieve the state of amplitude compensation mode.
Parameter:	None
Response:	(String) ALL or OUTPUT or NONE

AMPL_EMFOUT

Description:	Select EMF output mode.
Parameter:	ON or OFF
Restrictions:	Rejected during sweep.

Table 5B-3. Remote Commands (cont)

AMPL_EMFOUT?	
Description:	Retrieve the state of EMF output mode.
Parameter:	None
Response:	(String) ON or OFF
AMPL_MANUAL	
Description:	Increment or decrement the active manual amplitude sweep by specified number of counts. Note that the sign of sweep width affects the outcome of this operation.
Parameter:	Number of counts to increment or decrement the active manual amplitude sweep.
Restrictions:	Only allowed during manual amplitude sweep.
AMPL_RANGE	
Description:	Select amplitude range mode.
Parameter:	NORMAL or FIXED
Restrictions:	Rejected during sweep.
AMPL_RANGE?	
Description:	Retrieve the state of amplitude range mode.
Parameter:	None
Response:	(String) NORMAL or FIXED
AMPL_REL	
Description:	Select relative amplitude mode. Refer to Section 4B, "RF Amplitude" for more details.
Parameter:	ON or OFF
Restrictions:	Rejected during sweep.
AMPL_REL?	
Description:	Retrieve the state of relative amplitude mode.
Parameter:	None
Response:	(String) ON or OFF
AMPL_SINCR	
Description:	Program the amplitude sweep increment in dB or V. The default units are DB.
Parameter:	Increment with optional DB units or voltage units.
Restrictions:	Rejected during manual or single sweep.

Table 5B-3. Remote Commands (cont)

AMPL_SINCR?

Description: Retrieve the amplitude sweep increment.

Parameter: None

Responses:
1. (Float) Amplitude sweep increment.
2. (String) DB, V, or V-EMF

AMPL_STEP

Description: Program the amplitude step size in dB or V. The default units are DB.

Parameter: Amplitude step size with optional DB units or voltage units.

Restrictions: Rejected during manual or single sweep.

AMPL_STEP?

Description: Retrieve the amplitude step size.

Parameter: None

Responses:
1. (Float) Amplitude step size.
2. (String) DB, V, or V-EMF

AMPL_SWIDTH

Description: Program the amplitude sweep width in dB or V. The default units are DB. Note that a negative value will cause a sweep from a higher power level to a lower one.

Parameter: Sweep width with optional DB units or voltage units.

Example:
AMPL_SWIDTH –1.820E–6 V
AMPL_SWIDTH 10.2 DB
AMPL_SWIDTH 2

Restrictions: Rejected during manual or single sweep.

AMPL_SWIDTH?

Description: Retrieve the amplitude sweep width.

Parameter: None

Responses:
1. (Float) Amplitude sweep width.
2. (String) DB, V, or V-EMF

AMPL_UNITS

Description: Convert the AMPLITUDE display to specified units.

Parameter: DBM or V

Restrictions: Rejected during sweep.

Table 5B-3. Remote Commands (cont)

ATT_LOG?

Description:	Retrieve the attenuator log.
Parameter:	None
Responses:	1. (Integer) A6 attenuator count. 2. (Integer) A12 attenuator count. 3. (Integer) A24A attenuator count. 4. (Integer) A24B attenuator count. 5. (Integer) A24C attenuator count. 6. (Integer) A24D attenuator count. 7. (Integer) A24E attenuator count.
Example:	1470,1180,641,627,607,587,577

BRT_FIELD

Description:	Move the bright digit to the specified field.
Parameter:	AM or AMPL or FM or FREQ or MODF or MODL
Restrictions:	Rejected during sweep.

BRT_FIELD?

Description:	Retrieve the current bright-digit field.
Parameter:	None
Response:	(String) AM or AMPL or FM or FREQ or MODF or MODL

CAL_AM

Description:	Initiate AM calibration procedure. Note that the rear panel CAL|COMP switch must be set to 1 (on).
Parameter:	None
Restrictions:	Rejected during a calibration or compensation procedure, or during sweep.

CAL_FM

Description:	Initiate FM calibration procedure. Note that the rear panel CAL|COMP switch must be set to 1 (on).
Parameter:	None
Restrictions:	Rejected during a calibration or compensation procedure, or during sweep.

CAL_LEVEL

Description:	Initiate level calibration procedure. Note that the rear panel CAL|COMP switch must be set to 1 (on).
Parameter:	None
Restrictions:	Rejected during a calibration or compensation procedure, or during sweep.

Table 5B-3. Remote Commands (cont)

CAL_REFOSC

Description:	Initiate reference oscillator calibration procedure. Note that the rear panel CAL|COMP switch must be set to 1 (on).
Parameter:	None
Restrictions:	Rejected during a calibration or compensation procedure, or during sweep.

CC_ERRFREQ?

Description:	Returns error code and frequency where automatic comp procedure failed. If no errors were generated, a zero is returned for both the error code and frequency responses.
Parameter:	None
Responses:	1. (Integer) Error Code 2. (Float) Frequency 3. (String) HZ

CC_EXIT

Description:	Exit calibration/compensation procedure.
Parameter:	None
Restrictions:	Only allowed when performing a calibration or compensation procedure.

CC_FREQ?

Description:	Retrieve the RF output frequency during calibration/ compensation procedure.
Parameter:	None
Responses:	1. (Float) Output frequency 2. (String) HZ
Restrictions:	Only allowed when performing a calibration procedure or attenuator, output, or subsynthesizer compensation procedure.

CC_HETADJ?

Description:	Returns Het band frequency and level adjustments where Het level adjustment can be made following an unsuccessful output compensation procedure. If no output compensation procedure has been performed since power-on, a zero is returned for both frequency and adjustment responses.
Parameter:	None
Responses:	1. (Float) Frequency 2. (String) HZ 3. (Float) Level Adjustment 4. (String) DB

CC_RDAM

Description:	Report measured AM depth to calibration procedure. Default units are PCT.
Parameter:	AM depth with optional PCT or % units.
Restrictions:	Only allowed when performing an AM calibration procedure.

Table 5B-3. Remote Commands (cont)

CC_RDDVM

Description:	Report measured voltage to compensation procedure. Default units are V.
Parameter:	Voltage with optional voltage units.
Restrictions:	Only allowed when performing a sub-synthesizer compensation procedure.

CC_RDFM

Description:	Report measured FM deviation to calibration procedure. Default units are HZ.
Parameter:	FM deviation with optional frequency units.
Restrictions:	Only allowed when performing an FM calibration procedure.

CC_RDFREQ

Description:	Report measured RF frequency to calibration procedure. Default units are HZ.
Parameter:	Frequency with optional frequency units.
Restrictions:	Only allowed when performing a reference oscillator calibration procedure.

CC_RDPOWER

Description:	Report measured power to calibration/compensation procedure. Default units are DBM.
Parameter:	Output power with optional DBM units.
Restrictions:	Only allowed when performing a level calibration or attenuator or output compensation procedure.

CC_SAVE

Description:	Calculate corrections, save new data in calibration/compensation memory. Note that the rear panel CAL|COMP switch must be set to 1 (on).
Parameter:	None
Restrictions:	Only allowed when performing a calibration procedure or attenuator, output, or subsynthesizer compensation procedure.

CC_TARGET?

Description:	Return target value of calibration/compensation procedure.
Parameter:	None
Responses:	1. (Float): Target value. 2. (String) PCT, HZ, DBM, or V
Restrictions:	Only allowed when performing a calibration procedure or attenuator, output, or subsynthesizer compensation procedure.

***CLS**

Description:	Clear status. Clears the ESR, the ISCR, and the error and status queues. Terminates a pending operation complete command (*OPC or *OPC?).
Parameter:	None

Table 5B-3. Remote Commands (cont)

CMEM_FIX

Description: Repair calibration/compensation memory checksum errors. Note that the rear panel CAL|COMP switch must be set to 1 (on).

Parameter: None

Restrictions: Rejected during a calibration or compensation procedure, or during sweep.

COMP_ATT

Description: Initiate attenuator compensation procedure. Note that the rear panel CAL|COMP switch must be set to 1 (on).

Parameter: None

Restrictions: Rejected during a calibration or compensation procedure, or during sweep.

COMP_COARSE

Description: Initiate automatic coarse loop compensation procedure. Note that the rear panel CAL|COMP switch must be set to 1 (on).

Parameter: None

Restrictions: Rejected during a calibration or compensation procedure, or during sweep.

COMP_OUT

Description: Initiate output compensation procedure. Note that the rear panel CAL|COMP switch must be set to 1 (on).

Parameter: None

Restrictions: Rejected during a calibration or compensation procedure, or during sweep.

COMP_OUTDEF

Description: Initiate output compensation procedure with default attenuator through-path corrections applied. Note that the rear panel CAL|COMP switch must be set to 1 (on).

Parameter: None

Restrictions: Rejected during a calibration or compensation procedure, or during sweep.

COMP_SUBSYN

Description: Initiate subsynthesizer compensation procedure. Note that the rear panel CAL|COMP switch must be set to ON.

Parameter: None

Restrictions: Rejected during a calibration or compensation procedure, or during sweep.

COMP_SUM

Description: Initiate automatic sum loop compensation procedure. Note that the rear panel CAL|COMP switch must be set to 1 (on).

Parameter: None

Restrictions: Rejected during a calibration or compensation procedure, or during sweep.

Table 5B-3. Remote Commands (cont)

***DDT**

Description: Define device trigger. Used to load commands into the device trigger buffer for subsequent execution when a *TRG common command or the group execute trigger (GET) IEEE-488.1 interface message is received. The syntax of the data loaded is not checked until the trigger command is received. A *TRG command in the trigger buffer will cause an Execution Error when the trigger command is received.

Parameter: #0<user data><ASCII Line Feed with EOI>
or
#<non-zero digit><digits><user data>

For both forms, the bytes received in the <user data> field are stored in non-volatile memory and up to 72 bytes are allowed. The first form accepts data bytes after the #0 until the ASCII Line Feed character is received with an EOI signal.

In the second form, the non-zero digit specifies the number of characters that will follow in the <digits> field. These characters must be 0 through 9 (ASCII 48 through 57 decimal). The value of the number in the <digits> field defines the number of user data bytes that will follow in the <user data> field.

Examples: *DDT #0STEP_FREQ UP<Line Feed with EOI>
or
*DDT #212STEP_FREQ UP

NOTE

The 2 indicates that there are two digits to follow (in this case "12"), and the 12 indicates that there are twelve characters in the remainder of the *DDT message (in this case, "STEP_FREQ UP").

***DDT?**

Description: Retrieves the contents of the *DDT (Define Device Trigger) buffer.

Parameter: None

Response: #<non-zero digit><digits><user data>

The non-zero digit specifieds the number of characters that will follow in the <digits> field. These characters are 0 through 9 (ASCII 48 through 57 decimal). The value of the number in the <digits> field defines the number of user data bytes that follow in the <user data> field. The maximum response is 72 characters.

Example: #212STEP_FREQ UP

DISPLAY

Description: Select the display status.

Parameter: ON or OFF

Table 5B-3. Remote Commands (cont)

DISPLAY?

Description:	Retrieve the display status.
Parameter:	None
Response:	(String) ON or OFF

EDIT_AM

Description:	Select the AM bright-digit field and edit AM by the specified number of counts.
Parameter:	Number of counts by which bright digit is edited.
Example:	AM_BRT 1 PCT; EDIT_AM -18
Restrictions:	Rejected during manual or single sweep.

EDIT_AMPL

Description:	Select the amplitude bright-digit field and edit amplitude by the specified number of counts.
Parameter:	Number of counts by which bright digit is edited.
Example:	EDIT_AMPL 293
Restrictions:	Rejected during manual or single sweep.

EDIT_FM

Description:	Select the FM bright-digit field and edit FM by the specified number of counts.
Parameter:	Number of counts by which bright digit is edited.
Restrictions:	Rejected during manual or single sweep.

EDIT_FREQ

Description:	Select the frequency bright-digit field and edit frequency by the specified number of counts.
Parameter:	Number of counts by which bright digit is edited.
Example:	FREQ_BRT 1 HZ; EDIT_FREQ 172
Restrictions:	Rejected during manual or single sweep.

EDIT_MODF

Description:	Select the modulation frequency bright-digit field and edit modulation frequency by the specified number of counts.
Parameter:	Number of counts by which bright digit is edited.
Restrictions:	Rejected during manual or single sweep.

EDIT_MODL

Description:	Select the modulation level bright-digit field and edit modulation level by the specified number of counts.
Parameter:	Number of counts by which bright digit is edited.
Restrictions:	Rejected during manual or single sweep.

Table 5B-3. Remote Commands (cont)

ERROR?

Description:	Retrieve earliest error code from the error queue. If no error codes are pending, a zero is returned. If the optional keyword EXPLAIN is specified, a character string containing its explanation is returned with the error code.
Parameter:	(optional) EXPLAIN
Examples:	FREQ 100 GHZ; ERROR? EXPLAIN Returns: 1,"Frequency out of range" FREQ 100 GHZ; ERROR? Returns: 1
Responses:	1. (Integer) The error code. 2. (optional) (String) The explanation of the code.

***ESE**

Description:	Loads a byte into the Event Status Enable Register, described under "Checking the Instrument Status".
Parameter:	The decimal equivalent of the binary number to load into the register (0-255 only).
Example:	*ESE 140 Enables bits 2 (QYE), 3 (DDE), and 7 (PON), and disables all the other bits. (See "Checking the Instrument Status" for details.)

***ESE?**

Description:	Retrieves the byte from the Event Status Enable register, described under "Checking the Instrument Status".
Parameter:	None
Response:	(Integer) Decimal equivalent of the register byte.
Example:	*ESE? Returns: "140" if bits 2 (QYE), 3 (DDE), and 7 (PON) are enabled (1) and the rest of the bits are disabled (0). (See "Checking the Instrument Status" for details.)

***ESR?**

Description:	Retrieve the byte from the Event Status Register and clears the register. The ESR is described under "Checking the Instrument Status".
Parameter:	None
Response:	(Integer) Decimal equivalent of the register byte.
Example:	*ESR? Returns: "140" if bits 2 (QYE), 3 (DDE), and 7 (PON) are set (1) and the rest of the bits are reset (0). (See "Checking the Instrument Status" for details.)

Table 5B-3. Remote Commands (cont)

ETIME?

Description:	Retrieve the elapsed time. This gives the time (with tenths-of-hours resolution) that the Signal Generator has been in operation since it was manufactured.
Parameter:	None
Responses:	1. (Float) Total number of hours the instrument has been operating. 2. (String) HRS
Example:	5058.7,HRS

EXPLAIN?

Description:	Explain a status/error code. This command returns a string which is the explanation of the status or error code furnished as the parameter. The controller will most likely obtain the code via the STATUS? or ERROR? query. Refer to Appendices C, D, and E for a list of status and error codes.
Parameter:	The error/status code to explain.
Response:	(String) The explanation of the code.
Example:	EXPLAIN? 1 Returns: "Frequency out of range"

EXT_PULSE

Description:	Turn external pulse modulation On or Off.
Parameter:	ON or OFF
Restrictions:	Rejected during single sweep.

EXT_PULSE?

Description:	Retrieve the state of external pulse modulation.
Parameter:	None
Response:	(String) ON or OFF

EXTAC_AM

Description:	Turn external AM (AC coupled) On or Off
Parameter:	ON or OFF
Restrictions:	Rejected during single sweep.

EXTAC_AM?

Description:	Retrieve the state of external AM (AC coupled).
Parameter:	None
Response:	(String) ON or OFF

EXTAC_FM

Description:	Turn external FM (AC/ØM coupled) On or Off.
Parameter:	ON or OFF
Restrictions:	Rejected during single sweep.

Table 5B-3. Remote Commands (cont)

EXTAC_FM?

Description:	Retrieve the state of external FM (AC/ØM coupled).
Parameter:	None
Response:	(String) ON or OFF

EXTDC_AM

Description:	Turn external AM (DC coupled) On or Off.
Parameter:	ON or OFF
Restrictions:	Rejected during single sweep.

EXTDC_AM?

Description:	Retrieve the state of external AM (DC coupled).
Parameter:	None
Response:	(String) ON or OFF

EXTDC_FM

Description:	Turn external DCFM/DCØM On or Off.
Parameter:	ON or OFF
Restrictions:	Rejected during single sweep.

EXTDC_FM?

Description:	Retrieve the state of external DCFM/DCØM.
Parameter:	None
Response:	(String) ON or OFF

EXTREF_FREQ

Description:	Select the external reference frequency.
Parameter:	STD (10 MHz) ALT (Refer to Section 4A, "RF Frequency")
Restrictions:	Rejected during sweep.

EXTREF_FREQ?

Description:	Retrieve the selected external reference frequency.
Parameter:	None
Response:	(String) STD or ALT

FM

Description:	Program the FM/ØM deviation in Hz or radians. The default units are HZ.
Parameter:	FM/ØM deviation with optional frequency or radians units.
Restrictions:	Rejected during manual or single sweep.

Table 5B-3. Remote Commands (cont)

FM?

Description:	Retrieve the FM/ØM deviation.
Parameter:	None
Responses:	1. (Float) FM/ØM deviation. 2. (String) HZ or RAD

FM_BRT

Description:	Move the bright digit to the specified decade in FM/ØM field. Note that the unit must match the displayed units (e.g. HZ, KHZ, MHZ, or GHZ for Hz; RAD for Radians) when specifying the bright-digit position. The default units are HZ.
Parameter:	Bright-digit decade in FM/ØM display field with optional frequency or radians units.
Example:	FM_BRT 10.0 KHZ
Restrictions:	Rejected during manual or single sweep.

FM_BRT?

Description:	Retrieve the decade of FM/ØM bright-digit position.
Parameter:	None
Responses:	1. (Float) Bright-digit decade in FM/ØM display. 2. (String) HZ or RAD

FM_RANGE

Description:	Select normal mode or low distortion or fixed range FM.
Parameter:	NORMAL or LOWDISTORT or FIXED
Restrictions:	Rejected during sweep.

FM_RANGE?

Description:	Retrieve the state of low distortion or fixed range FM.
Parameter:	None
Response:	(String) NORMAL or LOWDISTORT or FIXED

FM_STEP

Description:	Program the FM/ØM deviation step size in Hz or radians. The default units are HZ.
Parameter:	FM/ØM deviation step size with optional frequency or radians units.
Example:	FM_STEP 13.26 KHZ
Restrictions:	Rejected during manual or single sweep.

Table 5B-3. Remote Commands (cont)

FM_STEP?

Description:	Retrieve the FM/ØM deviation step size.
Parameter:	None
Responses:	1. (Float) FM deviation step size. 2. (String) HZ or RAD

FM_UNITS

Description:	Convert the FM/ØM display to specified units.
Parameter:	HZ or RAD
Restrictions:	Rejected during manual or single sweep.

FREQ

Description:	Program the displayed RF frequency in Hz. The default units are HZ. If FREQ_REL is OFF, this is the RF output frequency. Refer to Section 4A, "RF Frequency" for more details. If If Auto Frequency Sweep is active, programs the center Frequency. Refer to Section 4E, "Sweep" for more information.
Parameter:	Frequency with frequency units.
Example:	FREQ 183.277281 MHZ
Restrictions:	Rejected during manual or single sweep.

FREQ?

Description:	Retrieve the displayed RF frequency. If FREQ_REL is OFF, this is the RF output frequency. If Frequency Sweep is active, returns the center Frequency. Refer to Section 4E, "Sweep" for more information.
Parameter:	None
Responses:	1. (Float) Displayed RF frequency. 2. (String) HZ
Example:	1.832772810E+08,HZ

FREQ_ABS?

Description:	Retrieve the RF output frequency.
Parameter:	None
Responses:	1. (Float) Output RF frequency. 2. (String) HZ

FREQ_BASE?

Description:	Retrieve the base frequency. If FREQ_REL is OFF, this value is 0. Refer to Section 4A, "RF Frequency" for more details.
Parameter:	None
Responses:	1. (Float) Base RF frequency. 2. (String) HZ

Table 5B-3. Remote Commands (cont)

FREQ_BRT	
Description:	Move the bright digit to specified decade in frequency field. The default units are HZ.
Parameter:	Bright-digit decade in FREQUENCY display field with optional frequency units.
Example:	FREQ_BRT 10.0 KHZ
Restrictions:	Rejected during manual or single sweep.
FREQ_BRT?	
Description:	Retrieve the decade of frequency bright-digit position.
Parameter:	None
Responses:	1. (Float) Bright-digit decade in FREQUENCY display. 2. (String) HZ
FREQ_MANUAL	
Description:	Increment or decrement the active manual frequency sweep by specified number of counts. Note that the sign of sweep width affects the outcome of this operation.
Parameter:	Number of counts to increment or decrement the active manual frequency sweep.
Restrictions:	Only allowed during manual frequency sweep.
FREQ_REL	
Description:	Select relative frequency mode. Refer to Section 4A, "RF Frequency" for more details.
Parameter:	ON or OFF
Restrictions:	Rejected during sweep.
FREQ_REL?	
Description:	Retrieve the state of relative frequency mode.
Parameter:	None
Response:	(String) ON or OFF
FREQ_SINCR	
Description:	Program the frequency sweep increment in Hz. The default units are HZ.
Parameter:	Sweep increment with optional frequency units.
Example:	FREQ_SINCR 123.322 KHZ
Restrictions:	Rejected during manual or single sweep.

Table 5B-3. Remote Commands (cont)

FREQ_SINCR?

Description:	Retrieve the frequency sweep increment.
Parameter:	None
Responses:	1. (Float) Frequency sweep increment. 2. (String) HZ
Example:	1.233220000E+05,HZ

FREQ_STEP

Description:	Program the frequency step size in Hz. The default units are HZ.
Parameter:	Frequency step size with optional frequency units.
Restrictions:	Rejected during manual or single sweep.

FREQ_STEP?

Description:	Retrieve the frequency step size.
Parameter:	None
Responses:	1. (Float) Frequency step size. 2. (String) HZ
Example:	3.002300000E+08,HZ

FREQ_SWIDTH

Description:	Program the frequency sweep width in Hz. The default units are HZ. Note that a negative value will cause a sweep from a higher frequency to a lower frequency.
Parameter:	Sweep width with optional frequency units.
Example:	FREQ_SWIDTH –9.634 KHZ
Restrictions:	Rejected during manual or single sweep.

FREQ_SWIDTH?

Description:	Retrieve the frequency sweep width.
Parameter:	None
Responses:	1. (Float) Frequency sweep width. 2. (String) HZ
Example:	–9.634000000E+03,HZ

GAL

Description:	Go to alternate language (the specified language is "remembered" when the power is turned off). See Section 5D, "Compatibility Languages".
Parameter:	L6080 or L6070 or L6060 or L8642

Table 5B-3. Remote Commands (cont)

HIRATEPM

Description:	Turn high rate ØM mode On or Off.
Parameter:	ON or OFF
Restrictions:	Rejected during sweep.

HIRATEPM?

Description:	Retrieve the state of the high rate ØM mode.
Parameter:	None
Response:	(String) ON or OFF

***IDN?**

Description:	Retrieve instrument identification.
Parameter:	None
Responses:	1. (String) FLUKE 2. (String) Model 3. (String) Serial Number 4. (String) Firmware Level
Example:	FLUKE,6080A,12345678,V1.0

INT_AM

Description:	Turn internal AM On or Off.
Parameter:	ON or OFF
Restrictions:	Rejected during single sweep.

INT_AM?

Description:	Retrieve the state of internal AM.
Parameter:	None
Response:	(String) ON or OFF

INT_FM

Description:	Turn internal FM/ØM On or Off.
Parameter:	ON or OFF
Restrictions:	Rejected during single sweep.

INT_FM?

Description:	Retrieve the state of internal FM/ØM.
Parameter:	None
Response:	(String) ON or OFF

Table 5B-3. Remote Commands (cont)

INT_PULSE

Description:	Turn internal pulse modulation On or Off.
Parameter:	ON or OFF
Restrictions:	Rejected during single sweep.

INT_PULSE?

Description:	Retrieve the state of internal pulse modulation.
Parameter:	None
Response:	(String) ON or OFF

ISCE

Description:	Loads a byte into the Instrument Status Change Enable register described under the "Checking the Instrument Status".
Parameter:	The decimal equivalent of the binary number to load into the register.
Example:	ISCE 56
	Enables bits 3 (RPP), 4 (FM LO), and 5 (FM HI) in the Service Request Enable register.

ISCE?

Description:	Retrieves the byte from the Instrument Status Change Enable register, described under "Checking the Instrument Status".
Parameter:	None
Response:	The decimal equivalent of the register contents byte.
Example:	ISCE?
	Returns: "4" if bit 3 (RPP) is enabled (1) and the rest of the bits are disabled (0). (See "Checking the Instrument Status" for details.)

ISCR?

Description:	Retrieves and clears the byte from the Instrument Status Change Register, described under "Checking the Instrument Status".
Parameter:	None
Response:	The decimal equivalent of the register contents byte.
Example:	ISCR?
	Returns: "8" if bit 3 (RPP) is set (1) and the rest of the bits are reset (0). (See "Checking the Instrument Status" for details.)

Table 5B-3. Remote Commands (cont)

ISR?

Description:	Retrieves and clears the byte from the Instrument Status Register, described under "Checking the Instrument Status".
Parameter:	None
Response:	The decimal equivalent of the register contents byte.
Example:	ISR?
	Returns: "16" if bit 4 (FM LO) is set (1) and the rest of the bits are reset (0). (See "Checking the Instrument Status" for details.)

KEY_RATE

Description:	Select the repeat rate for the step keys.
Parameter:	SLOW or MEDIUM or FAST
Restrictions:	Rejected during sweep.

KEY_RATE?

Description:	Retrieve the key repeat rate.
Parameter:	None
Response:	(String) SLOW or MEDIUM or FAST

KNOB_STEP

Description:	Select the operation of the knob and step up/down keys. The knob can be turned on (default) or off, the step up/down keys can be configured to perform step up/down function (default) or edit up/down function.
Parameters:	1. ON or OFF (Turns the knob on or off) 2. STEP or EDIT (Configures the step keys)
Example:	KNOB_STEP OFF, EDIT (Knob off, step keys do edits)
Restrictions:	Rejected during sweep.

KNOB_STEP?

Description:	Retrieve the state of the knob and step up/down keys.
Parameter:	None
Responses:	1. (String) ON or OFF 2. (String) STEP or EDIT
Example:	OFF,EDIT (Knob off, step keys do edits)

LOCALERT

Description:	Set mode to generate an SRQ on complete front panel operations.
Parameter:	ON or OFF

Table 5B-3. Remote Commands (cont)

LOCALERT?

Description:	Retrieve the state of the local alert (LOCALERT) mode.
Parameter:	None
Response:	(String) ON or OFF

LORATEFM

Description:	Turn low rate FM mode On or Off.
Parameter:	ON or OFF
Restrictions:	Rejected during sweep.

LORATEFM?

Description:	Retrieve the state of the low rate FM mode.
Parameter:	None
Response:	(String) ON or OFF

MEM_DIVIDER

Description:	Program memory divider locations for sequence operations.
Parameter:	1. Memory divider 1 location number 2. Memory divider 2 location number 3. Memory divider 3 location number 4. Memory divider 4 location number
Example:	MEM_DIVIDER 5, 23, 45, 30
Restrictions:	Rejected during sweep.

MEM_DIVIDER?

Description:	Retrieve memory divider locations for sequence operations.
Parameter:	None
Responses:	1. (Integer) Memory divider 1 location number 2. (Integer) Memory divider 2 location number 3. (Integer) Memory divider 3 location number 4. (Integer) Memory divider 4 location number
Example:	5,23,30,45

MEM_LOCK

Description:	Set lock protection for memory store.
Parameter:	ON or OFF
Restrictions:	Rejected during sweep.

MEM_LOCK?

Description:	Retrieve the state of memory lock protection.
Parameter:	None
Response:	(String) ON or OFF

Table 5B-3. Remote Commands (cont)

MEM_RESET

Description:	Reset all memory locations to the default instrument state (memory location 98).
Parameter:	None
Restrictions:	Rejected during sweep.

MOD_DISPLAY

Description:	Select the quantity to be shown in the modulation field of the display. This command does not move the bright digit.
Parameter:	AM or FM or MODF or MODL
Restrictions:	Rejected during manual or single sweep.

MOD_DISPLAY?

Description:	Retrieve the quantity shown in the modulation field Note that a value will be returned even though the display may be turned off with the DISPLAY command.
Parameter:	None
Response:	(String) AM or FM or MODF or MODL

MOD_WAVE

Description:	Select the output waveform for the modulation oscillator.
Parameter:	SINE or TRIANGLE or SQUARE or PULSE
Restrictions:	Rejected during sweep.

MOD_WAVE?

Description:	Retrieve the modulation oscillator waveform.
Parameter:	None
Response:	(String) SINE or TRIANGLE or SQUARE or PULSE

MODF

Description:	Program the modulation frequency in Hz. The modulation frequency may be programmed with 0.1 Hz resolution. The default units are HZ.
Parameter:	Modulation frequency with optional frequency units.
Example:	MODF 100.0001 KHZ
Restrictions:	Rejected during manual or single sweep.

MODF?

Description:	Retrieve the modulation frequency.
Parameter:	None
Responses:	1. (Float) Modulation frequency. 2. (String) HZ
Example:	1.000001000E+05,HZ

Table 5B-3. Remote Commands (cont)

MODF_BRT

Description:	Move the bright digit to specified decade in modulation frequency field. The default units are HZ.
Parameter:	Bright-digit decade in modulation frequency display field with optional frequency units.
Example:	MODF_BRT 1.0 KHZ
Restrictions:	Rejected during manual or single sweep.

MODF_BRT?

Description:	Retrieve the decade of modulation frequency bright-digit position.
Parameter:	None
Responses:	1. (Float) Bright-digit decade in modulation frequency display. 2. (String) HZ

MODF_STEP

Description:	Program the modulation frequency step size in Hz. The default units are HZ.
Parameter:	Modulation frequency step size with optional frequency units.
Restrictions:	Rejected during manual or single sweep.

MODF_STEP?

Description:	Retrieve the modulation frequency step size.
Parameter:	None
Responses:	1. (Float) Modulation frequency step size. 2. (String) HZ

MODL

Description:	Program the modulation level in volts. The default units are V.
Parameter:	Modulation level with optional voltage units.
Examples:	MODL 1 MODL 100 MV
Restrictions:	Rejected during manual or single sweep.

MODL?

Description:	Retrieve the modulation level.
Parameter:	None
Responses:	1. (Float) Modulation level. 2. (String) V
Example:	1.000E–01,V

Table 5B-3. Remote Commands (cont)

MODL_BRT

Description:	Move the bright digit to specified decade in modulation level field. The default units are V.
Parameter:	Bright-digit decade in modulation level display field with optional voltage units.
Example:	MODL_BRT 1.0 V
Restrictions:	Rejected during manual or single sweep.

MODL_BRT?

Description:	Retrieve the decade of modulation level bright-digit position.
Parameter:	None
Responses:	1. (Float) Bright-digit decade in modulation level display. 2. (String) V

MODL_STEP

Description:	Program the modulation level step size in volts. The default units are V.
Parameter:	Modulation level step with optional voltage units.
Restrictions:	Rejected during manual or single sweep.

MODL_STEP?

Description:	Retrieve the modulation level step size.
Parameter:	None
Responses:	1. (Float) Modulation level step size. 2. (String) V

MODOUT

Description:	Select the state of the MOD OUTPUT port.
Parameter:	ON (modulation output always at output port) OFF (modulation output port is off)
Restrictions:	Rejected during sweep.

MODOUT?

Description:	Retrieve the state of the MOD OUTPUT port.
Parameter:	None
Response:	(String) ON or OFF

Table 5B-3. Remote Commands (cont)

***OPC**

Description: Programs bit 0 (OPC for "Operation Complete") in the Event Status Register to 1 when all pending device operations are complete. The Signal Generator considers an operation complete according to the following rules.

- The operation is complete when the command is processed and output has settled.
- For those commands that do not change the output, the operation is complete when the command is processed.
- Single sweep is complete when the sweep is complete. The operation is not complete when sweep is turned off before the sweep completes.
- Auto and manual sweep command are complete when the starting frequency/amplitude has been programmed and the output has settled.
- Automatic calibration/compensation procedures are complete when the procedure is complete. The operation is not complete when the procedure is aborted.
- Other calibration/compensation procedures are complete when the first step has been programmed and the output has settled.

Parameter: None

***OPC?**

Description: Returns a 1 after all pending operations are complete. This commands causes program execution to pause until all operations are complete. (See also *WAI.)

Parameter: None

Response: (Integer) "1" after all operations are complete.

***OPT?**

Description: Retrieve report of installed options.

Parameter: None

Responses: (Series of strings) A comma-separated list of the option names. Each option name includes the option number and a description. If the option is not installed, a zero is returned instead of the string.

Examples: -130 High Stability Reference,-830 Rear Output
0,-830 Rear Output

PHASE

Description: Adjust the phase of the rf carrier.

Parameter: (Float) Phase adjustment (in degrees).

Restrictions: Rejected during sweep.

Table 5B-3. Remote Commands (cont)

PHASE?

Description: Retrieve the relative phase adjustment.

Parameter: None

Response: (Float) Relative phase adjustment.

PHASE_CLK

Description: Program the measured phase adjustment clock frequency. Note that the rear panel CAL|COMP switch must be set to 1 (on).

Parameter: 1. (Float) Clock frequency
2. (String) Hz

Restrictions: Rejected during sweep.

PHASE_CLK?

Description: Retrieve the phase adjustment clock frequency.

Parameter: 1. (Float) Clock frequency
2. (String) Hz

PHASE_ZERO

Description: Zero the relative phase adjustment.

Parameter: None

Restrictions: Rejected during sweep.

PRESET

Description: Reset instrument to preset state. See Appendix A, "Instrument Preset State".

Parameter: None

***PUD**

Description: Define protected user data data. This command allows you to store a string of bytes in non-volatile memory. This command works only when the CAL|COMP switch is in the 1 (on) position.

Parameter: #0 <user data> <ASCII Line Feed with EOI>
or
#<non-zero digit> <digits> <user data>

For both forms, the bytes received in the <user data> field are stored in nonvolatile memory and up to 63 bytes are allowed. The first form accepts data bytes after the #0 until the ASCII Line Feed character is received with an EOI signal.

In the second form, the non-zero digit specifies the number of characters that will follow in the <digits> field. These characters must be 0 through 9 (ASCII 48 through 57 decimal). The value of the number in the <digits> field defines the number of user data bytes that will follow in the <user data> field.

Table 5B-3. Remote Commands (cont)

Examples: Store the word "FLUKE" in the protected user data area:

*PUD #0FLUKE<Line Feed with EOI>
or
*PUD #15FLUKE

NOTE

The 1 indicates that there is one digit to follow (in this case,"5"), and the 5 indicates that there are five characters in the remainder of the *PUD message (in this case, "FLUKE").

***PUD?**

Description: Retrieve protected user data buffer.

Parameter: None

Response: #(non-zero digit) (digits) (user data)

The non-zero digit specifies the number of characters that will follow in the <digits> field. These characters are 0 through 9 (ASCII 48 through 57 decimal). The value of the number in the <digits> field defines the number of user data bytes that follow in the <user data> field. The maximum response is 64 characters.

Example: *PUD?

Returns: "205FLUKE" assuming that this is stored as in the example for PUD* above.

PULSE_WIDTH

Description: Program the modulation oscillator pulse width for the variable width pulse waveform in seconds. Default units are S.

Parameter: Pulse width with optional seconds units.

Example: PULSE_WIDTH 40.0 US

Restrictions: Rejected during sweep.

PULSE_WIDTH?

Description: Retrieve the modulation oscillator pulse width.

Parameter: None

Responses: 1. (Float) Pulse width.
2. (String) S

Example: 4.000000000E–05,S

***RCL**

Description: Recall a memory location. This command allows the user to recover the programmed instrument state from the specified memory location (contents of which are loaded by the *SAV command).

Parameter: Memory location.

Restrictions: Rejected during sweep.

Table 5B-3. Remote Commands (cont)

REF?

Description:	Retrieve the state of the frequency reference selection.
Parameter:	None
Response:	(String) INT or EXT

RFOUT

Description:	Turns the RF output port On or Off.
Parameter:	ON or OFF

RFOUT?

Description:	Retrieve the state of the RF output port.
Parameter:	None
Response:	(String) ON or OFF

***RST**

Description:	Reset instrument to default memory location. The default memory location is 97 (See Appendix A, "Instrument Preset State"). In addition to the recall of location 97, sweep is turned off, and any current calibration or compensation procedures are aborted. No other actions are performed on the *RST command.
Parameter:	None

***SAV**

Description:	Save (store) to a memory location. This command allows a user to store the current instrument programmed state in a specified memory location for later retrieval by the *RCL command.
Parameter:	Memory location.
Restrictions:	Rejected during sweep.

SD

Description:	Step the active step field down by one step size.
Parameter:	None
Restrictions:	Rejected during single sweep.

SEQ

Description:	Recall the next or previous memory location.
Parameter:	UP or DOWN
Restrictions:	Rejected during sweep.

Table 5B-3. Remote Commands (cont)

SPCL

Description: Select a special function by number.

Parameter: Special function number.

***SRE**

Description: Program the Service Request Enable register (SRE), described under "Checking the Instrument Status".

Parameter: The decimal equivalent of the binary number to load into the register.

Example: *SRE 56

Enables bits 3 (IIR), 4 (MAV), and 5 (ESR) in the Service Request Enable register.

***SRE?**

Description: Retrieve Service Request Enable register, described in under the heading "Checking the Instrument Status".

Parameter: None

Response: (Integer) The decimal equivalent of the register byte.

Example: *SRE?

Returns: "56" if bits 3 (IIR), 4 (MAV), and 5 (ESR) are enabled (1) and the rest of the bits are disabled (0). (See "Checking the Instrument Status" for details.)

STATUS

Description: Load specified status into the status queue. Uncal, self-test, memory checksum, and memory origin status can be loaded.

Parameter: UNCAL or SELFTEST or CHECKSUM or ORIGIN

STATUS?

Description: Retrieve a status code from the status queue. If no status codes have been loaded with the STATUS command or if all the enqueued status codes have been retrieved, a zero is returned. If the optional keyword EXPLAIN is specified, a character string containing its explanation is returned with the status code.

Parameter: (optional) EXPLAIN

Examples:

STATUS?
Returns: 220 (If the RPP has tripped)

STATUS? EXPLAIN
Returns: 220, "RPP tripped" (If the RPP has tripped)

Responses:

1. (Integer) Currently loaded uncal, self-test, or memory status code, or a zero.
2. (optional) (String) The explanation of the code.

Table 5B-3. Remote Commands (cont)

***STB?**

Description:	Retrieve the status byte. The status byte is described in under the heading "Checking the Instrument Status".
Parameter:	None
Response:	(Integer) Decimal equivalent of the status byte.
Example:	*STB?
	Returns: "72" if bits 3 (EAV) and 6 (MSS) are set (1) and the rest of the bits are reset (0).

STEP_AM

Description:	Step the AM depth up or down by one step size.
Parameter:	UP or DOWN
Restrictions:	Rejected during single sweep.

STEP_AMPL

Description:	Step the output amplitude up or down by one step size.
Parameter:	UP or DOWN
Restrictions:	Rejected during single sweep.

STEP_FIELD

Description:	Program the specified field to be used for the step up/down functions.
Parameter:	AM or AMPL or FM or FREQ or MODF or MODL
Restrictions:	Rejected during manual or single sweep.

STEP_FIELD?

Description:	Retrieve the current step field.
Parameter:	None
Response:	(String) AM or AMPL or FM or FREQ or MODF or MODL

STEP_FM

Description:	Step the FM/øM deviation up or down by one step size.
Parameter:	UP or DOWN
Restrictions:	Rejected during single sweep.

STEP_FREQ

Description:	Step the output frequency up or down by one step size.
Parameter:	UP or DOWN
Restrictions:	Rejected during single sweep.

Table 5B-3. Remote Commands (cont)

STEP_MODF

Description:	Step the modulation frequency up or down by one step size.
Parameter:	UP or DOWN
Restrictions:	Rejected during single sweep.

STEP_MODL

Description:	Step the modulation level up or down by one step size.
Parameter:	UP or DOWN
Restrictions:	Rejected during single sweep.

SU

Description:	Step the active step field up by one step size.
Parameter:	None
Restrictions:	Rejected during single sweep.

SWEEP

Description:	Select the sweep mode.
Parameter:	OFF or AUTO or MANUAL or SINGLE

SWEEP?

Description:	Retrieve the sweep mode.
Parameter:	None
Response:	(String) OFF or AUTO or MANUAL or SINGLE

SWEEP_DWELL

Description:	Program the sweep dwell time. Default units are S.
Parameter:	Dwell time with optional seconds units.
Example:	SWEEP_DWELL 500 MS

SWEEP_DWELL?

Description:	Retrieve the sweep dwell time.
Parameter:	None
Responses:	1. (Integer) Dwell time. 2. (String) S

SWEEP_FIELD

Description:	Select the sweep field.
Parameter:	FREQ (Frequency) AMPL (Amplitude)
Restrictions:	Rejected during sweep.

Table 5B-3. Remote Commands (cont)

SWEEP_FIELD?

Description:	Retrieve the sweep field.
Parameter:	None
Response:	(String) FREQ or AMPL

SWEEP_SYM

Description:	Select the sweep symmetry.
Parameter:	ASYM (Asymmetrical) SYMM (Symmetrical)
Restrictions:	Rejected during single sweep.

SWEEP_SYM?

Description:	Retrieve the sweep symmetry.
Parameter:	None
Response:	(String) ASYM or SYMM

TEST_ATT

Description:	Program alternate attenuator settings.
Parameter:	A24B or A24C or A24D or A24E
Restrictions:	Rejected during sweep.

TEST_DISP

Description:	Execute display test.
Parameter:	ON or OFF
Restrictions:	Rejected during sweep.

***TRG**

Description:	Trigger device. Cause the commands defined with the *DDT common command to be executed. If the *DDT has been specified with a zero-length data block, no action will be taken.
Parameter:	None

***TST?**

Description:	Initiates a series of self-tests, then returns a "0" for pass or a "1" for fail. If any tests fail, they can be loaded into the status queue with the STATUS SELF-TEST command. The enqueued status codes can be queried with the STATUS? command. Refer to the Service Manual for a description of tests performed.
Parameter:	None
Response:	(Integer) 0 (for Pass) or 1 (for Fail)
Restrictions:	Turns sweep or calibration or compensation procedure off.

Table 5B-3. Remote Commands (cont)

***WAI**

Description:	Wait until all pending remote operations are complete. This command prevents further remote commands from being executed until all previous remote commands have been completely executed.
Parameter:	None

Section 5C
Talk-Only/Listen-Only Operation

INTRODUCTION 5C-1.

The Signal Generator can be used with any IEEE-488 controller in the normal addressed mode. The listen-only and talk-only modes are available for operation without a controller.

In the listen-only mode, the Signal Generator responds to all data messages on the IEEE-488 bus. In the talk-only mode, the Signal Generator sends commands on the IEEE-488 bus to program another Signal Generator.

TALK-ONLY OPERATION 5C-2.

In talk-only, the Signal Generator outputs the step up (";SU") and step down (";SD") commands whenever the front panel step up and down entries are made.

Two Signal Generators can be set up to track in frequency with an offset by connecting one Signal Generator in talk-only to another Signal Generator in listen-only. This is done by: programming the two signal generators to the desired frequencies; programming the frequency step value to be the same on both generators; and pressing the step up or step down keys on the generator that is in talk-only mode. Note that if the step sizes are different or if the functions selected to step are different, the signal generators will no longer track with the same offset.

Any of the six functions may be stepped (frequency, amplitude, AM depth, FM deviation, modulation frequency, and modulation level), and the step function of the talker need not match that of the listener.

A Fluke 6060A, 6060B, 6061A, or 6062A may also be used as the listener with the limitation that they cannot step modulation frequency or modulation level. A Fluke 6070A or 6071A may be used as the listener with the limitation that it will always step frequency.

The 6080A and 6082A implement the talk-only (ton) function described in the IEEE-488.1 standard. The IEEE-488.2 standard does not cover talk-only operation.

The talk-only mode is selected by the talker/listener special function described in Section 5, "Remote Operation". When the mode is changed, the IEEE-488 interface chip is reset, and any current IEEE-488 bus activity is discarded. In talk-only, the signal generator is always in local, and is always addressed as a talker. The ADDR annunciator is always be lit.

In talk-only, the device clear, trigger, and serial poll messages are ignored.

LISTEN-ONLY OPERATION 5C-3.

A Fluke 6060A, 6060B, 6061A, or 6062A may be used as a talk-only instrument with a 6080A or 6082A as the listener. They output ",SU" and ",SD" which will cause a command error for the 6080 language. Therefore, if the 6080A or 6082A is to be the listener, it should be configured to one of the compatibility languages as described in Section 5, "Remote Operation".

The Signal Generator implements the listen-only (lon) function described in the IEEE-488.1 standard. The IEEE-488.2 standard does not cover listen-only operation.

The listen-only mode is selected by the talker/listener special function described in Section 5, "Remote Operation". When the mode is changed, the IEEE-488 interface chip is reset, and any current IEEE-488 bus activity is discarded. In listen-only, the signal generator is always in local, and is always addressed as a listener. The ADDR annunciator is always lit.

In listen-only, the Signal Generator will respond to all commands that are allowed with the exception of queries and calibration/compensation commands. These commands will be processed with no errors, but nothing will be sent over the bus.

In listen-only, device clear, trigger, and serial poll messages will be ignored.

LISTEN-ONLY/TALK-ONLY EXAMPLE 5C-4.

The Signal Generator can be connected to another Signal Generator in a master-slave configuration. In the following example, two Signal Generators are configured to track each other in frequency. This configuration may be used to track frequency, amplitude, AM, FM, Modulation Frequency or Modulation Level.

1. Connect two Signal Generators together with an IEEE-488 cable.

2. Set the talker/listener mode of the first Signal Generator (talker) to talk-only by entering [SPCL] [1] [1], then entering [1] in response to the prompt.

3. Set the talker/listener mode of the second Signal Generator (listener) by entering [SPCL] [1] [1], then entering [2] in response to the prompt.

4. Manually program the talker Signal Generator as follows:

FUNCTION	VALUE	KEY SEQUENCE
Frequency	210 MHz	[FREQ] [2] [1] [0] [MHz|V]
Step Function	Frequency	[FREQ] [STEP]
Frequency Step	1.25 kHz	[1] [.] [2] [5] [kHz|mV]

5. Manually program the listener Signal Generator as follows:

FUNCTION	VALUE	KEY SEQUENCE
Frequency	195 MHz	FREQ 1 9 5 MHz/V
Step Function	Frequency	FREQ STEP
Frequency Step	1.25 kHz	1 . 2 5 kHz/mV

6. On the talker Signal Generator, press the △ STEP or ▽ STEP keys. Each time the key is pressed, the frequency of both Signal Generators increases or decreases by 1.25 kHz (the Frequency Step) at frequencies 15 MHz apart.

Different functions on each Signal Generator can be programmed to track in the master-slave configuration. In other words, while the master Signal Generator can be programmed to step increase 25 kHz FM, the slave Signal Generator can be programmed to step 25% AM.

NOTE

To use the step feature for other functions, change the step function on the Signal Generators to the desired functions.

Section 5D
Compatibility Languages

INTRODUCTION 5D-1.

The previous programming information in Sections 5A through 5C all relates to the default (6080) remote language, which complies with the IEEE-488.2 standard. Use the default language for all new applications.

The Signal Generator can also be configured to respond to commands intended for Fluke Models 6060A, 6060B, 6061A, 6062A, 6070A, or 6071A, or Hewlett Packard Models 8642A or 8642B in an existing program. In this mode, the Signal Generator no longer complies with the IEEE-488.2 standard. The information in this sub-section describes the three compatibility languages built into Models 6080A and 6082A:

- Fluke 6060 family language
- Fluke 6070 family language
- HP8462 family language

The language setting is stored in non-volatile memory and is retained when the power is turned off.

SELECTING THE ACTIVE LANGUAGE 5D-2.

Enter [SPCL] [1] [2] to display the current IEEE-488 language in the FREQUENCY display field.

Enter [0] for the 6080 or default language (6080A or 6082A), [1] for the 6060 (6060A, 6060B, 6061A, or 6062A), [2] for the 6070 (6070A or 6071A), or [3] for the 8642 (HP8642A or B) language. Your language selection is displayed for about 2 seconds.

Use the GAL command to select the active language from remote. GAL without arguments will switch to the 6080 language from any language. When in the 6080, language arguments to the GAL command are L6060, L6070, L6080, and L8642. For example, to put the Signal Generator in the 6070 language, send the following programming string: "GAL; GAL L6070".

Some commands do not exist in the compatibility languages. To access 6080A/82A functions not supported in a compatibility language, you can intersperse 6080 commands with compatibility commands by inserting appropriate GAL commands. For example, the compatibility languages do not include queries. Send the command string "FR 100 HZ; GAL; FREQ?; GAL L6070" to temporarily switch to the 6080 language from the 6070 language to query the frequency.

USING THE 6060 AND 6070 FAMILY LANGUAGES 5D-3.

Once you have set the Signal Generator so that the 6060 or 6070 remote language is active, the Signal Generator is ready to operate in an existing 6060 or 6070 family system, but with some minor restrictions and differences. Use following text to help you decide on whether or not to make program modifications, and what to modify.

Incompatibilities 5D-4.

Most of the operations are identical to the 6060 and 6070 signal generators when using the compatibility language. A few minor differences do exist and are described in the following paragraphs.

The instrument limits and specifications are those of the 6080A/82A. For example, the frequency limits are 10 kHz to 1056 MHz for the FR command, even though the 6070A frequency limits are 200 kHz to 520 MHz.

The timing of programming and data transfer on the IEEE-488 bus will not be the same. The 6080A/82A will generally be faster than the 6060 family and slower than the 6070 family of products.

Status, rejected entry, and self-test codes are similar but not exactly the same. Those codes that are the same will be reported as they are in the 6060 or 6070 instruments. Most special functions for the 6060 and 6070 instruments are available in the 6080A/82A and the compatibility language will accept the 6060 or 6070 codes. Tables 5D-1 and 5D-2 list the codes and special functions for the 6060 and 6070 compatibility languages.

Three of the interface modes (record, unbuffered, and valid) have been replaced with the interrogate complete (IP) and wait (WA) commands. Refer to the 6080 language commands *OPC? and *WAI for a description of their operation.

The response to the IO command will be the code for the 6080A/82A, not the compatibility instrument. For example, the response "12,0,0" indicates that the instrument is a 6080A with no options.

The bit values in the serial poll status byte are defined differently. However, two copies of the enable register and the status byte are maintained so that if only status codes available for the 6060 or 6070 are used, the SRQ line will not change when switching languages.

Some commands that are not commonly used have been eliminated in the compatibility language. Most of these are available in the 6080 language and can always be accessed by switching languages. Table 5D-3 shows the 6060 and 6070 commands supported in the compatibility languages. Some commands are listed as being available only for the 6080. These are for features such as programmable modulation level that are not available in the 6060 or 6070.

In the 6060 and 6070 instruments, numeric data can be sent in hexadecimal as well as the default decimal. This feature is not included in the 6060 and 6070 compatibility languages, but a similar capability is available in the 6080 language.

Table 5D-1. 6060 Compatibility Language Codes and Special Functions

RETURNED IN 6060 MODE	EQUIVALENT 6080 STATUS	DESCRIPTION
Status (value returned on 6060 IU command)		
000001,000000,000000	222	FM DAC at 0
000002,000000,000000	224	FM out of range for RF frequency band
000004,000000,000000	*	Excess FM Deviation
000010,000000,000000	223	FM DAC at full scale
000020,000000,000000	*	AM depth too high
000200,000000,000000	250	Multiple compensation memory errors
000000,000010,000000	246	Reference unlocked
000000,000000,000001	*	Level DAC below calibrated range
000000,000000,000002	*	Peak (AM) amplitude too high
000000,000000,000004	241	ALC loop unleveled
000000,000000,000010	220	Level DAC at 0
000000,000000,000020	221	Level DAC at full scale
000000,000000,000040	240	RPP tripped
000000,000000,000100	*	Amplitude too low
000000,000000,000200	201	Level correction disabled
000000,000000,000400	*	RF output off
001000,000000,000000	**	All other codes new for 6082A
Rejected entry (value returned on "IR" command)		
000001,000000,000000	30	FM/ØM deviation out of range
000002,000000,000000	31	FM/ØM step size out of range
000004,000000,000000	20	AM depth out of range
000010,000000,000000	21	AM step size out of range
000020,000000,000000	73	IEEE bad command syntax
000040,000000,000000	74	IEEE bad argument value
000100,000000,000000	98	MEC PROM ID code invalid, or MEC PROM checksum error
000200,000000,000000	71	IEEE invalid edit or step
000400,000000,000000	97	Stored cal/comp data has invalid data point
000000,000001,000000	1	Frequency out of range
000000,000002,000000	90,95	CALCOMP switch not set to 1 (on)
000000,000004,000000	2	Frequency step size out of range
000000,000010,000000	92	Cal/comp procedure incomplete, data cannot be stored
000000,000020,000000	94	Invalid cal/comp command
000000,000040,000000	61	Invalid memory location
000000,000100,000000	62	Memory location data invalid
000000,000200,000000	60	Invalid special function code
000000,000400,000000	93	Cal/comp data range error (too much correction)
000000,000000,000001	10	Amplitude out of range
000000,000000,000002	11	Amplitude unit conversion out of range
000000,000000,000004	12	Units conversion not allowed with voltage reference
000000,000000,000020	13	Amplitude step size out of range
000000,000000,000040	15	Amplitude step units conversion not allowed
000000,000000,000100	14	Amplitude step with mixed units not allowed
000000,000000,000200	91	Cal/comp out of range adjustment
000000,000000,000400	96	Internal cal/comp data transfer error
001000,000000,000000	**	All other rejected entry codes new for 6082A

Table 5D-1. 6060 Compatibility Language Codes and Special Functions (cont)

RETURNED IN 6060 MODE	EQUIVALENT 6080 STATUS	DESCRIPTION
Self-test (value returned on 6060 IT command)		
000,000,000,000		All tests passed
777,777,777,777		Some tests failed. Go to the 6080 language to query the results.
000,-000,000,000		Tests were aborted.
777,-777,777,777		Some tests failed and tests were aborted.
SENT IN 6060 MODE	**EQUIVALENT 6080 CODE**	**DESCRIPTION**
Special function (value sent with 6060 SP command)		
00	00	Clears special functions
02	02	Initiates power-on self-tests
03	*	Display test.
04	*	Button test.
07	14	Set front panel SRQ
08	15	Clear front panel SRQ
09	*	Display software revision level
10	*	Display IEEE-488 address and talker/listener mode
11	*	Display self-test results
12,13	770,771	Disable display
14	*	Initialize memory locations
15	*	Latch test.
16	*	Display option loading status
17	*	Initiate self-tests with RF output enabled
20,21	20,21	Relative frequency
30,31	30,31	Relative amplitude.
40,41	740,741	Internal pulse modulation
50-52	840-842	Select amplitude display units
60,61	****	DCAM
70-72	860-862	Select repeat rate for step keys
75	*	Display cal/comp memory checksum status and data origins
76	*	Repair cal/comp memory checksum errors
77-79	*	Transfer MEC Prom Data
80-82	920-922	Apply amplitude compensation
83-86	923-926	Program alternate 24 dB attenuators
90,91	50,51	Amplitude fixed range
95-98	*	Manual compensation procedures

NOTES:
*Feature not available for the Signal Generator, rejected for special functions.
**Feature new for the Signal Generator, no equivalent code for the 6060.
*** Special function rejected, it is only available from the front panel.
**** Special function rejected, use "DA1" instead of "SP61, AE1" and "DA0" instead of "SP61, AE0".

Table 5D-2. 6070 Compatibility Language Codes and Special Functions

RETURNED IN 6070 MODE	EQUIVALENT 6080 STATUS	DESCRIPTION
Status (value returned on 6070 IU command)		
000001,000000,000000,000000	222	FM DAC at 0
000002,000000,000000,000000	224	FM out of range for RF frequency band
000004,000000,000000,000000	247	FM loop unlocked
000010,000000,000000,000000	*	ACFM deviation too high
000020,000000,000000,000000	223	FM DAC at full scale
000040,000000,000000,000000	*	Delay discriminator unleveled
000100,000000,000000,000000	*	ACFM deviation too high
000200,000000,000000,000000	*	DCFM deviation too high
000000,000001,000000,000000	*	Modulation frequency DAC too low
000000,000002,000000,000000	*	Modulation frequency DAC too high
000000,000004,000000,000000	*	FM deviation too high
000000,000020,000000,000000	*	AM depth too high
000000,000000,000001,000000	*	6071A frequency out of calibrated limits
000000,000000,000002,000000	*	Mod divider filters out of calibrated limits
000000,000000,000004,000000	*	Frequency out of calibrated limits
000000,000000,000010,000000	242	Sub synthesizer unlocked
000000,000000,000020,000000	*	Delay discriminator not ready
000000,000000,000040,000000	*	Excess FM deviation
000000,000000,000100,000000	246	Reference phase detector unlocked
000000,000000,000000,000001	*	Level DAC too low
000000,000000,000000,000002	*	Peak (AM) amplitude too high
000000,000000,000000,000004	241	ALC loop unleveled
000000,000000,000000,000010	220	Level DAC at 0
000000,000000,000000,000020	221	Level DAC at full scale
000000,000000,000000,000040	240	RPP tripped
000000,000000,000000,000100	*	Amplitude too low
000000,000000,000000,000200	201	Level correction disabled
001000,000000,000000,000000	**	All other status codes new for 6082A
Rejected entry (value returned on 6070 IR command)		
000001,000000,000000,000000	30	FM/ØM deviation out of range
000002,000000,000000,000000	*	DCFM not allowed when phase modulation enabled
000004,000000,000000,000000	*	Radians entry not allowed with DCFM enabled
000010,000000,000000,000000	32	FM/ØM units conversion not allowed when external FM enabled
000020,000000,000000,000000	33	FM/ØM units conversion out of ØM range
000040,000000,000000,000000	61	Invalid memory location
000100,000000,000000,000000	*	Invalid memory location for insert/delete operation
000200,000000,000000,000000	62	Memory location data invalid
000000,000001,000000,000000	20	AM depth out of range
000000,000002,000000,000000	40	Mod frequency out of range
000000,000004,000000,000000	60	Invalid special function code
000000,000010,000000,000000	73	IEEE bad command syntax
000000,000020,000000,000000	74	IEEE bad argument value
000000,000040,000000,000000	71	IEEE invalid edit or step

Table 5D-2. 6070 Compatibility Language Codes and Special Functions (cont)

RETURNED IN 6070 MODE	EQUIVALENT 6080 STATUS	DESCRIPTION
000000,000100,000000,000000	*	IEEE invalid bright digit value
000000,000200,000000,000000	*	Bright-digit cannot be enabled during sweep
000000,000000,000001,000000	1	Frequency out of range
000000,000000,000004,000000	2,3,4	Frequency step size/sweep width/sweep increment out of range
000000,000000,000010,000000	52	Entry conflicts with current sweep
000000,000000,000020,000000	51	Cannot enable sweep with current parameters
000000,000000,000000,000001	10	Amplitude out of range
000000,000000,000000,000002	11	Amplitude unit conversion out of range
000000,000000,000000,000004	12	Units conversion not allowed with voltage reference
001000,000000,000000,000000	**	All other rejected entry codes new for 6082A
Self-test (value returned on 6070 IT command)		
000000		All tests passed
777777		Some tests failed. Go to the 6080 language to query the results.
-000000		Tests were aborted.
-777777		Some tests failed and tests were aborted.
SENT IN 6070 MODE	**EQUIVALENT 6080 CODE**	**DESCRIPTION**
Special function (value sent with 6070 SP command)		
00	00	Clears all currently set stored special functions
01	***	Display special function status
02	02	Initiates the power-on self-tests
03	***	Display test.
04	***	Button test.
05	*	Pattern sensitive RAM check
06	*	Non-volatile memory check
07	14	Set SRQ
08	15	Reset SRQ
09	***	Display instrument software revision level.
10,11	****	Forced DCFM
20,21	*	Forced high deviation
30,31	50,51&730,732	Fixed range
40	890	Select sweep dwell time of 0 mS
41-44	891-895	Select sweep dwell time
50,51	880,881	Select sweep symmetry
60,61	*	Wideband reference
70,71	40,41	Modulation oscillator output
80,81	920,921	Apply amplitude compensation

NOTES:
*Feature not available for the Signal Generator, rejected for special functions.
**Feature new for the Signal Generator, no equivalent code for the 6060.
*** Special function rejected, it is only available from the front panel.
**** Special function rejected, use "DF1" instead of "SP11, FE1" and "DF0" instead of "SP11, AF0".

Table 5D-3. 6060 and 6070 Compatibility Language Commands

COMPAT. COMMAND	6080 COMMAND	DESCRIPTION	6070 & 6071	6060 & 6061	6062	6080
@	–	Set up interface modes	6070	6060	6062	
AB	AMPL_BRT	Position amplitude bright digit	6070	6060	6062	6080
AE	EXTAC_AM	Disable/enable external AM	6070	6060	6062	6080
AI	INT_AM	Disable/enable internal AM	6070	6060	6062	6080
AM	AM	Program AM depth	6070	6060	6062	6080
AN	AMPL_SINCR	Program amplitude sweep incr.				6080
AP	AMPL	Program amplitude	6070	6060	6062	6080
AS	SWEEP	Start (auto) sweep operation	6070			6080
AW	AMPL_SWIDTH	Program amplitude sweep width				6080
CB		Clear IEEE output buffer	6070	6060	6062	
CE	*CLS	Clear error status		6060	6062	6080
CL	PRESET	Device clear	6070	6060	6062	6080
CT	*DDT	Configure trigger buffer	6070	6060	6062	6080
DA	EXTDC_AM	Disable/enable external DCAM			6062	6080
DB	FM_BRT	Position FM bright digit	6070	6060	6062	6080
DD	STEP_FM	Step (down) FM		6060	6062	6080
DF	EXTDC_FM	Disable/enable external DCFM				6080
DQ	SEQ	Sequence (down) to next mem loc				6080
DS	FM_STEP	Program FM step		6060	6062	6080
DU	STEP_FM	Step (up) FM		6060	6062	6080
DW	–	Define RAM/ROM base address	6070	6060	6062	
EM	–	Disable/enable error mode		6060	6062	
FB	FREQ_BRT	Position frequency bright digit	6070	6060	6062	6080
FD	STEP_FREQ	Step (down) frequency		6060	6062	6080
FE	EXTAC_FM	Disable/enable external FM	6070	6060	6062	6080
FI	INT_FM	Disable/enable internal FM	6070	6060	6062	6080
FM	FM	Program FM deviation	6070	6060	6062	6080
FR	FREQ	Program frequency	6070	6060	6062	6080
FS	FREQ_STEP	Program frequency step	6070	6060	6062	6080
FU	STEP_FREQ	Step (up) frequency		6060	6062	6080
GAL	GAL	Go to alternate language				6080
IA	ATT_LOG?	Query attenuator log		6060	6062	6080
IB	–	Input I/O bit	6070	6060	6062	
ID	*IDN?	Query instrument ID	6070	6060	6062	6080
IE	ETIME?	Query elapsed time		6060	6062	6080
II	–	Query interface "@" modes		6060	6062	
IL	–	Query error log		6060	6062	
IM	*SRE?	Query status register enable	6070	6060	6062	6080
IO	*OPT?	Query option loading	6070	6060	6062	6080
IP	*OPC?	Query operation complete	6070	6060	6062	6080
IR	ERROR?	Query rejected entry status	6070	6060	6062	6080
IS	*IDN?	Query instrument serial number			6062	6080
IT	STATUS?	Query self-test status	6070	6060	6062	6080

Table 5D-3. 6060 and 6070 Compatibility Language Commands (cont)

COMPAT. COMMAND	6080 COMMAND	DESCRIPTION	6070 & 6071	6060 & 6061	6062	6080
IU	STATUS?	Query uncal status	6070	6060	6062	6080
IV	*IDN?	Query software version	6070	6060	6062	6080
KA	EDIT_AMPL	Edit amplitude	6070	6060	6062	6080
KB	–	Edit current bright digit field	6070	6060	6062	
KD	EDIT_FM	Edit FM deviation	6070	6060	6062	6080
KF	EDIT_FREQ	Edit frequency	6070	6060	6062	6080
KM	EDIT_MODF	Edit modulation frequency	6070			6080
KN	EDIT_MODL	Edit modulation level				6080
KP	EDIT_AM	Edit AM depth	6070	6060	6062	6080
LD	STEP_AMPL	Step (down) amplitude		6060	6062	6080
LS	AMPL_STEP	Program amplitude step		6060	6062	6080
LU	STEP_AMPL	Step (up) amplitude		6060	6062	6080
MB	MODF_BRT	Position mod freq bright digit	6070		6062	6080
MD	STEP_MODF	Step (down) modulation freq				6080
MF	MODF	Program modulation frequency	6070	6060	6062	6080
MI	MODF_STEP	Program modulation freq step				6080
ML	MODL	Program modulation level				6080
MR	–	Program mod freq to 400/1000 Hz		6060	6062	
MS	SWEEP	Start (manual) sweep operation	6070			6080
MU	STEP_MODF	Step (up) modulation freq				6080
NB	MODL_BRT	Position mod level bright digit				6080
ND	STEP_MODL	Step (down) modulation level				6080
NS	MODL_STEP	Program modulation level step				6080
NU	STEP_MODL	Step (up) modulation level				6080
OD	–	Output I/O DAC	6070	6060	6062	
PB	AM_BRT	Position AM bright digit	6070	6060	6062	6080
PD	STEP_AM	Step (down) AM depth		6060	6062	6080
PE	EXT_PULSE	Disable/enable external pulse			6062	6080
PH	PHASE	Program carrier phase adjustment				6080
PI	INT_PULSE	Disable/enable internal pulse			6062	6080
PS	AM_STEP	Program AM step		6060	6062	6080
PU	STEP_AM	Step (up) AM depth		6060	6062	6080
PW	PULSE_WIDTH	Program mod osc pulse width				6080
PZ	PHASE_ZERO	Zero relative phase adjustment				6080
RA	AMPL_REL	Disable/enable relative amplitude	6070	6060	6062	6080
RB	–	Query I/O byte	6070	6060	6062	
RC	*RCL	Recall memory location	6070	6060	6062	6080
RF	FREQ_REL	Disable/enable relative freq	6070	6060	6062	6080
RO	RFOUT	Turn RF output off/on	6070	6060	6062	6080
RW	–	Query I/O word	6070	6060	6062	
SD	SD	Step down	6070	6060	6062	6080
SF	SWEEP_FIELD	Select sweep field				6080

Table 5D-3. 6060 and 6070 Compatibility Language Commands (cont)

COMPAT. COMMAND	6080 COMMAND	DESCRIPTION	6070 & 6071	6060 & 6061	6062	6080
SI	FREQ_SINCR	Program freq sweep increment	6070			6080
SM	*SRE	Set service request enable	6070	6060	6062	6080
SO	SWEEP	Stop sweep operation	6070			6080
SP	SPCL	Program special functions	6070	6060	6062	6080
SQ	SEQ	Sequence (up) to next mem loc		6060	6062	6080
SS	SWEEP	Start (single) sweep operation	6070			6080
ST	*SAV	Save (store) memory location	6070	6060	6062	6080
SU	SU	Step up	6070	6060	6062	6080
SW	FREQ_SWIDTH	Program frequency sweep width	6070			6080
TM	–	Set terminator mode		6060	6062	
TR	*TRG	Trigger device	6070	6060	6062	6080
WA	*WAI	Wait until operation complete				6080
WB	–	Set I/O byte	6070	6060	6062	
WW	–	Set I/O word	6070	6060	6062	
XA		Query attenuator value	6070	6060	6062	
XB	–	Set attenuator value	6070	6060	6062	
XD	–	Program sub-synthesizer freq	6070	6060	6062	
XF	LOCALERT	Set local alert mode	6070	6060	6062	6080
XR	–	Fast RF on/off	6070	6060	6062	

Converting 6060 and 6070 Programs to Use the 6080 Language 5D-5.

Users of 6060 and 6070 instruments may wish to convert their programs to use the new features available in the 6080 language. The following paragraphs describe the differences between the compatibility language and the 6080 language to help with the conversion.

In the 6080 language, programming mnemonics are longer and more meaningful than the two-character commands in the compatibility language. A complete list is provided in Table 5D-3. All special functions are accessed mnemonically rather than with special function codes.

Device clear and the *RST command are defined by the IEEE–488.2 standard. The 6080 device clear is limited to clearing the input buffer and output queue and turning sweep and cal/comp procedures off. The *RST does a recall location 98 and clears the trigger buffer. In the compatibility language, the device clear clears the input and output queue and the equivalent of a CL command. The CL command clears the output queue, turns sweep and cal/comp procedures off, clears the trigger buffer, clears errors, turns the RF output on, and initializes the serial poll register enable and memory dividers.

A programming message syntax is defined by the IEEE-488.2 standard. There must be white space between the header and the numeric. This is not the case in the compatibility language. For example, "FM100HZ" is valid in the compatibility language but "FM 100HZ" is required in the 6080 language.

In the compatibility language, string terminators are defined to be comma and semicolon and are optional between programming commands. For example, "FM100HZSURO1" is equivalent to "FM100HZ,SU;RO1". In the 6080 language, comma is defined to be a data separator and is required between data elements. The semicolon is defined to be the message unit separator and is required between programming commands. For example, "FM 100 HZ; STEP_FM UP; RFOUT ON".

Units in the 6080 language are defined by the IEEE-488.2 standard and are not the same as the 6060 and 6070. Table 5D-4 lists the units in both languages.

The 6080 language uses parameters that are mnemonic such as ON and OFF to replace the 1 or 0 used in the compatibility language.

The IEEE-488.2 common command, *IDN? returns manufacturer, model, serial number, and software version number. This one command replaces the compatibility commands ID, IS, and IV.

A status response in the compatibility language was defined to include the terminator character. For example if the serial poll register enable (SRQ mask) is 134, the command "IM;IM"⟨terminator⟩ will return "134"⟨terminator⟩"134"⟨terminator⟩. In the 6080 language, multiple queries within one program message are separated by semicolons, and a terminator is sent at the end. For example, "*SRE?;*SRE?" ⟨terminator⟩ will return "134;134"⟨terminator⟩. In the compatibility language, the terminator is programmable, but in the 6080 language it is always linefeed with EOI asserted.

Table 5D-4. 6060 and 6070 Compatibility Language Units

UNIT NAME	COMPATIBILITY LANGUAGE	6080 LANGUAGE
Hertz	HZ	HZ
Kilohertz	KZ	KHZ
Megahertz	MZ	MHZ or MAHZ
Gigahertz	GZ	GHZ
dBm	DB	DBM or DBMW
dB	DB	DB
dBmV	-	DBMV
dBμV	-	DBUV
dBf	-	DBF or DBFW
Volt	V	V
Millivolt	MV	MV
Microvolt	UV	UV
Nanovolt	NV	NV
Percent	PC	PCT
Radian	RD	RAD
Second	SC	S

In the 6080 language, new programming commands cause previous query responses to be flushed from the output queue. In the compatibility language, the output queue is not flushed on new programming commands. For example, "*SRE?"⟨terminator⟩ "*SRE100"⟨terminator⟩ clears the *SRE? response, but "IM"⟨terminator⟩"SM100" ⟨terminator⟩ does not clear the IM response.

In the 6080 language, if a query but not a terminator is received and the status data is requested to be transferred to the IEEE-488 controller, an error is generated and the output queue is flushed. No error is generated in the compatibility language.

The bit values in the serial poll status byte are different. Refer to the "Checking the Instrument Status" in Section 5A.

After a syntax error, the 6080 language will ignore all characters until a terminator is found. The compatibility language will discard errors until a terminator, comma, or semicolon is found.

The interface modes (@ modes) have been replaced with the IEEE-488.2 common commands *OPC, *OPC?, and *WAI defined in the IEEE-488.2 standard. Refer to the heading "Using the *OPC?, *OPC, and *WAI Commands" in Section 5A. Languages for more information.

USING THE HP 8642 FAMILY LANGUAGE 5D-6.

Once you have set the Signal Generator so that the HP 8642 remote language is active, the Signal Generator is ready to operate in an existing HP 8642 family system, but with some minor restrictions and differences. Use following text to help you decide on whether or not to make program modifications, and what to modify.

IEEE-488 (GPIB) Address 5D-7.

The HP8642 allows a GPIB address to be set from 0 to 31, with address 31 designated as the "listen-only" state. The 6080A/82A allows any address from 0 to 30 to be set; "listen-only" is set exclusive of the GPIB address.

IEEE-488 (GPIB) Interface Capabilities 5D-8.

In the 8642 emulation mode, the 6080A/82A provides the following IEEE Std 488 capabilities consistent with the HP8642: SH1, AH1, TE0, L3, LE0, SR1, RL1, PP0, DC1, DT0, E2.

The 6080A/82A differs from the HP8642 in the capabilities listed in Table 5D-5.

Table 5D-5. IEEE-488 Interface Capibilities/HP8642 Language

FLUKE 6080A OR 6082A	HP8642
T5 - has talk-only mode C0 - no controller capability	T6 - no talk-only mode C1, C2 - controller C3, C28 capability

Data Input and Numeric Formatting 5D-9.

The HP8642 and the 6080A/82A in emulation mode handle input data the same way. When processing input, only the characters "a-z", "A-Z", "0-9", "+", ".", "?", and "-" are interpreted. Other characters, including space, line feed, and carriage return are ignored. Numeric data are limited to 10 digits of mantissa and 2 digits of exponent.

The HP8642 ignores data input over the bus while in local (REM unasserted). The Fluke 6080A/82A parses and executes input commands when in local.

Data Output 5D-10.

When addressed to talk, the HP8642 always has data available to be read. When in local, and unless a query command (OE, OA, etc) has been received, the display contents are presented. This feature is emulated by the 6080.

The HP8642 OC, OE, and OL queries are emulated. Their format consists of 2 fields: a numeric value, followed by an ASCII string. HP8642 syntax errors are reported as they are encountered, and programming errors recognized by the 6080A/82A are mapped to HP8642 message numbers as shown in Table 5D-6.

Since the 6080A/82A does not automatically change parameters based on a user action to change another parameter, the OC (Output Changed Parameter) query always generates a "0" response.

The OL (Output Hi/Low Status) query is fully emulated, as is the OA (Output Active Function) query.

As there are significant hardware differences between the 6080A/82A and the HP8642, the 6080A/82A emulation of the OH (Output Hardware Error) command is as follows: if a 6080A/82A hardware error or out-of-lock condition is detected, a "Fluke-Specific" Error Code is generated. You can then press the front panel [STATUS] key to determine the specific 6080A/82A hardware problem.

The HP8642 actions for Device Clear, Selected Device Clear, and Local Lockout are emulated in the 6080. The HP8642 Service Request generation, and clearing/setting of the RQS mask is emulated. Bits 0 and 7 of the Status Byte (End of Sweep and Parameter Changed) are always 0; if the corresponding bits of the RQS mask are set, no SRQ is generated.

HP8642 Commands that are Ignored 5D-11.

In the HP8642 emulation mode, the 6080A/82A interprets the entire HP8642 command set, though some commands are not implemented and cause no change to the 6080A/82A instrument state. When any of the commands in Table 5D-7 are received, error message 4098 - HP.CMD NOT EMULATED is generated.

RF Output Frequency 5D-12.

The HP8642 RF Frequency Programming capability is emulated except for the commands in Table 5D-8.

Table 5D-6. 6080 to HP8642 Error Code Mapping

HP8642 Message			Error Condition Detected in 6080
4001	"NEXT STEP NOT POSSIBLE	.E1"	"IEEE invalid edit or step"
4002	"NOT POSSIBLE.ABOVE MAX	.E2"	"Freq out of range"
4002	"NOT POSSIBLE.ABOVE MAX	.E2"	"Freq step size out of range"
4002	"NOT POSSIBLE.ABOVE MAX	.E2"	"Ampl out of range"
4002	"NOT POSSIBLE.ABOVE MAX	.E2"	"Ampl units conv out of range"
4002	"NOT POSSIBLE.ABOVE MAX	.E2"	"Ampl step size out of range"
4002	"NOT POSSIBLE.ABOVE MAX	.E2"	"AM depth out of range"
4002	"NOT POSSIBLE.ABOVE MAX	.E2"	"AM step size out of range"
4002	"NOT POSSIBLE.ABOVE MAX	.E2"	"FM/PM dev out of range"
4002	"NOT POSSIBLE.ABOVE MAX	.E2"	"FM/PM step size out of range"
4002	"NOT POSSIBLE.ABOVE MAX	.E2"	"Mod freq out of range"
4002	"NOT POSSIBLE.ABOVE MAX	.E2"	"Mod freq step size out of range"
4002	"NOT POSSIBLE.ABOVE MAX	.E2"	"Mod level out of range"
4002	"NOT POSSIBLE.ABOVE MAX	.E2"	"Mod level step out of range"
4023*	"MIXED AMPTD DISALLOWED	.E23"	"Ampl step with mixed units not allowed"
4037*	"MIXED FM/PM DISALLOWED	.E37"	"FM/PM step with mixed units not allowed"
4049	"FREQ.SWP+SWP.TIME LIMIT	.E49"	"Sweep cannot be enabled with current sweep parameters"
4052	"AP.SWP PREVENTS FR.SWP	.E52"	"Sweep field cannot be changed while sweeping"
4086	"INVALID SPCL FUNCTION	.E86"	"Special func code invalid"
4091*	"NO SAVE.MEMORY LOCKED	.E91"	"Store operation not allowed when Memory Locked"
4092	"SAVE/RECALL MAX = 50	.E92"	"Memory loction number invalid"
4093	"RECALL NOT DEFINED	.E93"	"Memory location data invalid"
4095	"ADRS VALID 0-30 ONLY	.E95"	"IEEE address must be <= 30"
4098*	"HP CMD. NOT EMULATED	.E98"	–
4099*	"FLUKE-SPECIFIC ERROR	.E99"	–

*These 4000-series numbers do not exist on the HP8642, but have been added to alert the user that the Signal Generator has detected an error.

Table 5D-7. HP8642 Commands That Are Ignored

COMMAND	DESCRIPTION
AA	Sweep Start Amplitude*
AB	Sweep Stop Amplitude*
BS	Backspace
EMOF	Turn EMF Mode Off
EMON	Turn EMF Mode On
EO	Entry Off
FA	Sweep Start Frequency*
FB	Sweep Stop Frequency*
HO	Help Off
HP	Help
KH	Knob Hold
KI	Knob Increment
KL	Move Cursor One Decade Left
KR	Move Cursor One Decade Right
MG	Message
RS	Reference Set
RCDN	Recall Down
RCUP	Recall Up
SA	Sweep Auto
SG	Sweep Single
SM	Sweep Manual
SH	Shift
SVDN	Save Down
SVUP	Save Up
ST	Sweep Time*

*Since these are active function codes, their function modifiers are also ignored (IS, UP, DN, ON, OF, KL, KR).

Table 5D-8. HP8642 RF Output Frequency Commands Not Accepted

COMMAND	HP SPECIAL FUNCTION	DESCRIPTION
SP8	8	Prefer HET Band
SP240	240	Decrement Frequency by 0.1 Hz
SP241	241	Increment Frequency by 0.1 Hz
SP250	250	Phase Adjustment from Knob and Step Up and Step Down Keys

Relative RF Frequency 5D-13.

The following HP8642 Relative RF Frequency commands are emulated:

- RZ (Turn On Relative Frequency Mode)
- RF (Turn Off Relative Frequency Mode)

The following commands are not emulated:

- RS <value> (Set Reference to a Specific Frequency)
- RSON (Set Reference to Last Selected Reference)
- RSOF (Turn Off Reference Frequency)

RF Frequency Sweep 5D-14.

The 6080A/82A does not emulate the HP8642 Frequency Sweep capability. Therefore, the commands in Table 5D-9 are not emulated.

Table 5D-9. Frequency Sweep Commands Not Accepted

COMMAND	DESCRIPTION
FA <value>	Set Frequency Sweep Start Point
FAON, FAOF	Turn On/Off Start Frequency
FAKL, FAKR	Start Frequency Cursor Left/Right
FAIS <value>	Start Frequency Increment Set
FAUP, FADN	Start Frequency Increment Up/Down
FB <value>	Set Frequency Sweep Stop Point
FBON, FBOF	Turn On/Off Stop Frequency
FBKL, FBKR	Stop Frequency Cursor Left/Right
FBIS <value>	Stop Frequency Increment Set
FBUP, FBDN	Stop Frequency Increment Up/Down
ST <value>	Set Sweep Time
STKL, STKR	Sweep Time Cursor Left/Right
STIS <value>	Sweep Time Increment Set
STUP, STDN	Sweep Time Increment Up/Down
SA	Sweep Auto
SG	Sweep Single
SM	Sweep Manual
SP119	Special Function 119 - Disable Settling
SP121	Special Function 121 - Sweep Up and Down
SP123	Special Function 123 - Phase Continuous Sweep

RF Output Amplitude 5D-15.

The HP8642 Amplitude Programming capability is fully emulated with the exception that the APUP and APDN commands are not allowed unless the Amplitude Increment and the displayed Amplitude are in consistent units (i.e. Volt-unit increment and Volt-unit display, or dB-unit increment and dB-unit display).

The 6080A/82A output ALC loop configuration provides isolation from outside intermodulation. Therefore, the following Special Functions are ignored, but generate no execution errors:

- SP4 (ALC Off)
- SP204 (ALC On)

EMF Units 5D-16.

The following HP8642 Amplitude EMF units commands are not emulated:

- EMOF (Turn Off EMF Mode)
- EMON (Turn On EMF Mode)

Relative Amplitude 5D-17.

The following HP8642 Relative Amplitude commands are emulated:

- RZ (Turn On Relative Amplitude Mode)
- RF (Turn Off Relative Amplitude Mode)

The following commands are not emulated:

- RS <value> (Set Reference to a Specific Amplitude)
- RSON (Set Reference to Last Selected Reference)
- RSOF (Turn Off Reference Amplitude)

Amplitude Sweep 5D-18.

The 6080A/82A does not emulate the HP8642 Amplitude Sweep capability. Therefore, the commands in Table 5D-10 are not emulated.

AM/Pulse Modulation 5D-19.

The 6080A/82A fully emulates the HP8642 AM and Pulse modulation functions.

FM/ϕM 5D-20.

The 6080A/82A does not support independent instances of ϕM and FM parameters. As a result, a displayed FM deviation will be converted its equivalent ϕM deviation and vice-versa if the complimentary parameter is selected. Apart from this, the 6080A/82A emulates the HP8642 FM and ϕM modulation functions except the commands in Table 5D-11.

Table 5D-10. Amplitude Sweep Commands Not Accepted

COMMAND	DESCRIPTION
AA <value>	Set Amplitude Sweep Start Point
AAON, AAOF	Turn On/Off Start Amplitude
AAKL, AAKR	Start Amplitude Cursor Left/Right
AAIS <value>	Start Amplitude Increment Set
AAUP, AADN	Start Amplitude Increment Up/Down
AB <value>	Set Amplitude Sweep Stop Point
ABON, ABOF	Turn On/Off Stop Amplitude
ABKL, ABKR	Stop Amplitude Cursor Left/Right
ABIS <value>	Stop Amplitude Increment Set
ABUP, ABDN	Stop Amplitude Increment Up/Down
SP122	Special Function 122 - Linear Amplitude Sweep

Table 5D-11. FM/ØM Commands Not Accepted

COMMAND	SPECIAL FUNCTION	DESCRIPTION
SP6	6	FM Pre-Emphasis On
SP114	114	FM Pre-Emphasis On
SP115	115	Negative ØM Polarity
SP116	116	DC FM Correction Off
SP117	117	DC FM Update Mode On
SP118	118	AC-Coupled DC FM On
SP119	119	Disable Settling

Internal Modulation Oscillator 5D-21.

The 6080A/82A Modulation Oscillator is digitally synthesized, and requires no calibration. Therefore, the following Special Functions are ignored, but generate no execution errors:

- SP113 (Modulation Frequency Correction Off)
- SP213 (Modulation Frequency Correction On)
- SP248 (Calibrate Modulation Frequency Bands)

NOTE

The 6080A/82A front panel MOD OUTPUT signal is in phase with the internal modulation signal. This is different from the 8642, where the two signals are 180 degrees out of phase.

Instrument Preset/Partial Preset 5D-22.

The 6080A/82A emulates the HP8642 Instrument Preset and Partial Preset states with the exception of the following parameters:

- Start Frequency
- Stop Frequency
- Start/Stop Frequency Increment
- Start/Stop Frequency Knob Increment
- Frequency Reference
- Start Amplitude
- Stop Amplitude
- Start/Stop Amplitude Increment
- Start/Stop Amplitude Knob Increment
- Amplitude Reference
- Amplitude Sweep Mode
- Sweep Time Increment
- Sweep Time Knob Increment

Knob Control/Entry Off 5D-23.

The 6080A/82A does not emulate the following HP8642 Knob Control commands:

- KI (Set Knob Increment)
- KHON (Knob Hold On)
- KHOF (Knob Hold Off)
- KL (Move Cursor One Decade Left)
- KR (Move Cursor One Decade Right)
- EO (Entry Off)

Step, Increment Set 5D-24.

The 6080A/82A emulates the 8642 Step and Increment Set functions with the exception of the following function prefixes:

- AA/AB (Start/Stop Amplitude)
- FA/FB (Start/Stop Frequency)
- ST (Sweep Time)

Save/Recall Register 5D-25.

The 6080A/82A emulates the HP8642 Save and Recall commands, with the following exceptions:

- RCUP (Recall Up)
- RCDN (Recall Down)
- SVUP (Save Up)
- SVDN (Save Down)

The following command is implemented differently in the 6080A/82A, in that the Instrument Preset State is stored in each memory location:

- SP251 (Special Function 251 - Clear Recall Registers)

The 6080A/82A does not emulate the HP8642 set sequence command:

- SS (Set Sequence)

Special Functions 5D-26.

A limited set of HP8642 Special Functions are emulated, as listed in Table 5D-12.

Messages 5D-27.

The following message/status command is not emulated:

- MG (Load Message Queue)

Table 5D-12. HP8642 Special Functions Emulated

COMMAND	DESCRIPTION
SP0	Turn Special Functions 4-9 Off
SP4	ALC Off*
SP5	External Low Rate FM
SP7	Low-Distortion FM
SP100	Turn Off All Specials < 200
SP112	Ext + Int Low Rate FM
SP113	Modulation Frequency Correction Off**
SP204	ALC On*
SP205	Turn Off External Low Rate FM
SP207	Turn Off Low-Distortion FM
SP212	Turn Off Ext + Int Low Rate FM
SP213	Modulation Frequency Correction On**
SP242	Phase Decrement 1 degree
SP243	Phase Increment 1 degree
SP244	Phase Decrement 5 degrees
SP245	Phase Increment 5 degrees
SP248	Calibrate Modulation Frequency Bands**
SP251	Clear All Recall Registers

* SP4, ALC Off and SP204, ALC On cause no change to the 6080A/82A instrument state, but cause no execution error. The 6080A/82A Output Circuit ALC loop is isolated.

** SP113, Mod Freq Correction Off, SP213 Mod Freq Correction On, and SP248 Calibrate Mod Freq Bands cause no change to the 6080A/82A instrument state, but cause no execution error. The 6080A/82A Modulation Oscillator is digitally synthesized and requires no calibration.

The Special Function Help commands are not emulated:

HP	Help
HO	Help Off

Appendix A
Instrument Preset State

Appendix A. Instrument Preset State

FUNCTION	SET TO STATES		
	SPCL 00	RCL 97 [1]	SPCL 01 [2] (PRESET)
FREQUENCY			
Output frequency		1000 MHz	1000 MHz
Relative frequency mode (SPCL 20)	Off	Off	Off
AMPLITUDE			
Output amplitude		–140 dBm	–140 dBm
RF output state			On
Relative amplitude mode (SPCL 30)	Off	Off	Off
Fixed range amplitude (SPCL 50)	Normal	Normal	Normal
Amplitude display units (SPCL 840)	dBm	dBm	dBm
EMF-Volts amplitude display mode (SPCL 850)	Off	Off	Off
MODULATION			
AM depth		30 %	30 %
FM/ØM deviation		5 kHz	5 kHz
Modulation frequency		1 kHz	1 kHz
Modulation level		0 V	0 V
Pulse width		500 µs	500 µs
Internal AM		Off	Off
External AC AM		Off	Off
External DC AM		Off	Off
Internal FM/ØM		Off	Off
External AC FM/ØM		Off	Off
External DC FM/ØM		Off	Off
External pulse modulation		Off	Off
Modulation Oscillator output (SPCL 40)	On	On	On
Low-rate FM (SPCL 710)	Off	Off	Off
High-rate ØM (SPCL 720)	Off	Off	Off
Low-distortion/fixed range FM (SPCL 730)	Normal	Normal	Normal
Internal pulse modulation (SPCL 740)	Off	Off	Off
Modulation oscillator waveform (SPCL 750)	Sine	Sine	Sine
SWEEP			
Frequency sweep width		100 MHz	100 MHz
Frequency sweep increment		1 MHz	1 MHz
Amplitude sweep width		10 dB	10 dB
Amplitude sweep increment		.1 dB	.1 dB
Active sweep field		Freq.	Freq.
Sweep dwell time (SPCL 890)	0 s	0 s	0 s
Sweep symmetry (SPCL 880)	Sym.	Sym.	Sym.
Sweep mode			Off
EDIT			
Frequency bright-digit		10 MHz	10 MHz
Amplitude bright-digit		10 dBm	10 dBm
AM bright-digit		10 %	10 %
FM bright-digit		1 kHz	1 kHz

Appendix A. Instrument Preset State (cont)

FUNCTION	SET TO STATES		
	SPCL 00	RCL 97 [1]	SPCL 01 [2] (PRESET)
Modulation frequency bright-digit		1 kHz	1 kHz
Modulation level bright-digit		100 mV	100 mV
Modulation display field		FM	FM
Active bright-digit field		Freq.	Freq.
STEP			
Frequency step size		10 MHz	10 MHz
Amplitude step size		10 dB	10 dB
AM depth step size		10 %	10 %
FM/øM deviation step size		1 kHz	1 kHz
Modulation frequency step size		1 kHz	1 kHz
Modulation level step size		.1 V	.1 V
Active step field		Freq.	Freq.
MISCELLANEOUS			
Display (SPCL 770)			On
Key repeat rate (SPCL 860)			Medium
Knob and step key operation (SPCL 870)			On, Step
Calibration/compensation procedures			Off
Amplitude compensation (SPCL 920)			All
REMOTE			
Service request enable (SPCL 13)			0
Event status enable			0
Instrument status change enable			0

NOTES:

1. *Store and recall operations include these parameters.*
2. *Power-on State.*

SPCL 00 and RCL 97 are not allowed while the Signal Generator is sweeping.

The following instrument parameters are only set from the Fluke factory or with their associated commands:

External reference frequency (SPCL 760)	*Standard*
Display (SPCL 770)	*On*
Memory dividers (SPCL 802)	*0,0,0,0*
Memory lock state (SPCL 810)	*Off*
Output compensation data (SPCL 930)	*Standard*
IEEE-488 address (SPCL 10)	*2*
IEEE-488 addressed/listen-only/talk-only (SPCL 11)	*Addressed*
IEEE-488 language (SPCL 12)	*6080 Language*

Appendix B
Special Function Table

Appendix B. Special Function Table

SPECIAL FUNCTION	DESCRIPTION
00	Clear special functions
01	Restore Instrument Preset State
02	Initiate power-on self tests
03	Display self test results
06	Selftests with rf and pulse tests
08	Display option loading status
09	Display software revision level
10	Display/Set IEEE-488 address
11	Display/Set IEEE-488 address mode
12	Display/Set IEEE-488 language
13	Display/Enter service request mask
14	Set user request SRQ
15	Clear SRQ
20	Disable relative frequency mode
21	Enable relative frequency mode
30	Disable relative amplitude mode
31	Enable relative amplitude mode
40	Enable modulation oscillator output
41	Disable modulation oscillator output
42	Enter modulation frequency with 0.1 Hz resolution
50	Disable fixed range amplitude
51	Enable fixed range amplitude
701	Enable phase adjust mode
702	Zero phase adjust indicator
710	Disable low-rate FM
711	Enable low-rate FM
720	Disable high-rate øM
721	Enable high-rate øM
730	Select normal range FM
731	Select low-distortion range FM
732	Select fixed range FM
740	Disable internal pulse modulation
741	Enable internal pulse modulation
750	Select Sine oscillator waveform
751	Select triangle oscillator waveform
752	Select square oscillator waveform
758	Select pulse waveform
759	Enter pulse width

Appendix B. Special Function Table (cont)

SPECIAL FUNCTION	DESCRIPTION
760	Use 10 MHz external reference input frequency
761	Use alternate external reference input frequency
770	Enable display
771	Disable display
801	Reset memory locations
802	Display/Set memory sequence dividers
810	Unlock memory store operations
811	Lock memory store operations
840	Select dBm amplitude display units
841	Select dBmV amplitude display units
842	Select dBuV amplitude display units
843	Select dBf amplitude display units
850	Disable EMF-Volts amplitude display mode
851	Enable EMF-Volts amplitude display mode
860	Select medium key repeat rate
861	Select fast key repeat rate
862	Select slow key repeat rate
870	Normal knob and step key operation
871	Knob disabled, normal step key operation
872	Normal knob, step keys operate as EDIT up/down
873	Knob disabled, step keys operate as EDIT up/down
880	Select symmetrical sweep symmetry
881	Select asymmetrical sweep symmetry
882	Initiate single sweep
890	Select sweep dwell time of 0 ms
891	Select sweep dwell time of 20 ms
892	Select sweep dwell time of 50 ms
893	Select sweep dwell time of 100 ms
894	Select sweep dwell time of 200 ms
895	Select sweep dwell time of 500 ms

Appendix B. Special Function Table (cont)

SPECIAL FUNCTION	DESCRIPTION
04	Display cal/comp memory checksum status
05	Display cal/comp memory data origins
901	Display test
902	Button test
903	Latch test
904	Initiate self tests with RF output enabled
905	Display operating time since manufacture in hours
907	Repair cal/comp memory checksum errors
908	Phase adjust clock
909	Diagnostic preset state
920	Enable amplitude compensation
921	Disable all amplitude compensation
922	Disable attenuator amplitude compensation
923	Program alternate A24b attenuator
924	Program alternate A24c attenuator
925	Program alternate A24d attenuator
926	Program alternate A24e attenuator
930	Use normal output compensation data
931	Use alternate output compensation data
941	Set all internal DACs to zero
942	Set all internal DACs to half scale
943	Set all internal DACs to full scale
945	Display sum loop frequency
946	Display coarse loop frequency
947	Display subsynthesizer frequency
961	Transfer output MEC prom data
962	Transfer attenuator MEC prom data
963	Transfer subsynthesizer MEC prom data
971	Automatic coarse loop compensation procedure
972	Automatic sum loop compensation procedure
981	Front panel output compensation procedure
982	Front panel attenuator compensation procedure
983	Front panel output compensation w/default attenuator procedure
984	Front panel subsynthesizer compensation procedure
991	Front panel AM calibration procedure
992	Front panel FM calibration procedure
993	Front panel level calibration procedure
994	Front panel reference oscillator calibration procedure

Appendix C
Rejected Entry Error Codes

Appendix C. Rejected Entry Error Codes

ERROR CODE	DESCRIPTION
	FREQUENCY
1	Frequency out of range
2	Frequency step size out of range
3	Frequency sweep width out of range
4	Frequency sweep increment out of range
	AMPLITUDE
10	Amplitude out of range
11	Amplitude units conversion out of range
12	Amplitude units conversion not allowed with voltage reference
13	Amplitude step size out of range
14	Amplitude step with mixed units not allowed
15	Amplitude step/sweep width/sweep increment units conversion not allowed
16	Amplitude sweep width out of range
17	Amplitude sweep increment out of range
	AM
20	AM depth out of range
21	AM step size out of range
	FM/øM DEVIATION
30	FM/øM deviation out of range
31	FM/øM step size out of range
32	FM/øM units conversion not allowed when external FM enabled
33	FM/øM units conversion out of range
34	FM/øM step with mixed units not allowed
35	FM/øM step units conversion not allowed
	MOD FREQUENCY / MOD LEVEL
40	Mod frequency out of range
41	Mod frequency step size out of range
42	Mod level out of range
43	Mod level step size out of range
44	Pulse width out of range
	SWEEP
50	Sweep field (Freq/Ampl) cannot be changed while sweeping
51	Sweep cannot be enabled with current sweep parameters
52	Entry conflicts with active sweep
53	Selected function not allowed while sweep is active
54	Amplitude sweep with mixed units not allowed
55	Selected function not allowed unless sweep is active

Appendix C. Rejected Entry Error Codes (cont)

ERROR CODE	DESCRIPTION
	SPECIAL FUNCTION AND MEMORY
60	Special function code invalid
61	Memory location number invalid
62	Memory location data invalid
63	Store operation not allowed when memory locked
69	Phase adjust clock frequency out of range
	REMOTE
70	IEEE address must be <= 30
71	IEEE invalid edit or step
72	IEEE invalid command
73	IEEE bad command syntax
74	IEEE bad argument value
75	IEEE bad argument type
76	IEEE bad argument count
77	IEEE invalid keyword
78	IEEE 488.2 unterminated command
79	IEEE 488.2 interrupted query
80	IEEE 488.2 I/O deadlock
81	IEEE error/status queue overflow
82	IEEE recursive trigger buffer not allowed
83	IEEE command not allowed in local mode
84	IEEE query after indefinite response
	CALIBRATION/COMPENSATION
90	CAL|COMP switch not set to 1 (on)
91	Cal/comp adjustment out of range
92	Cal/comp procedure incomplete, data cannot be stored
93	Cal/comp data range error (too much correction)
94	Command not allowed during current cal/comp procedure
95	Command only allowed with appropriate cal/comp procedure
96	Internal cal/comp data transfer error
97	Stored cal/comp memory contains invalid data
98	MEC PROM ID code invalid, or MEC PROM checksum error
99	Sum loop compensation procedure failed
100	Coarse loop compensation procedure failed

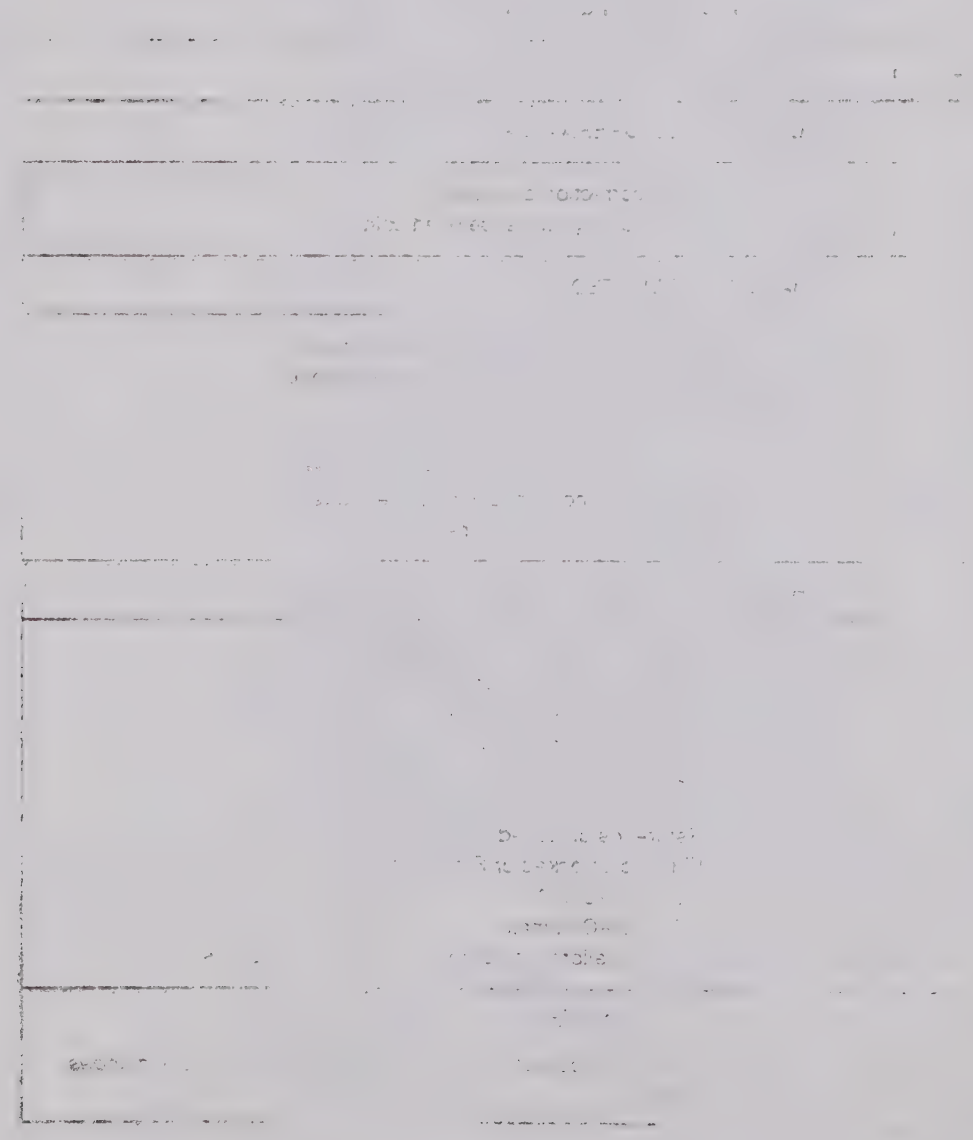

Appendix D
Overrange/Uncal Status Codes

Appendix D. Overrange/Uncal Status Codes

STATUS CODE	DESCRIPTION
UNSPECIFIED OPERATION	
201	Level correction disabled
202	High-stability reference oven cold
HARDWARE LIMITED	
220*	Level DAC at 0(Amplitude fixed range)
221*	Level DAC at max(Amplitude fixed range)
222*	FM DAC at 0 (FM fixed range)
223*	FM DAC at max (FM fixed range)
224*	FM out of range for RF frequency band
225*	Mod frequency too low for pulse mode
226*	Pulse width >= 1/mod frequency
HARDWARE FAULT	
240*	RPP tripped
241*	ALC loop unleveled or AM overmodulation
242*	Sub synthesizer unlocked
243*	Coarse loop unlocked
244*	Sum loop unlocked
245*	Sum loop unleveled
246*	Reference unlocked
247*	FM loop unlocked or FM overmodulation
248*	DCFM DAC at 0
249*	DCFM DAC at max
250*	Multiple calibration/compensation memory errors

NOTE:

*Flashing codes (denoted by *) indicate abnormal operation or aberrated output. Non-flashing codes indicate operation outside specified range.*

Appendix A. Self-Test Status Bits

Bit	Description
15	Master self-test error
14	Slave self-test error
13	Reserved
12	Reserved
11	Configuration/comparison memory checksum test failed
10	Reserved
9	EAROM test failed
8	Non-volatile memory test failed
7	RFE interface test failed
6	Reserved
5	Reserved
4	Reserved
3	Reserved
2	Reserved
1	Reserved
0	Reserved

Appendix E
Self-Test Status Codes

Appendix E. Self-Test Status Codes

STATUS CODE	DESCRIPTION
00	No self test errors
301	Self tests aborted
302	Calibration/compensation memory checksum test failed
303	Ram test failed
304	EPROM test failed
305	Non-volatile memory test failed
306	IEEE interface test failed
307-309	AM tests (See Service Manual)
310-317	FM tests (See Service Manual)
318-319	DCFM tests (See Service Manual)
320-323	Coarse loop tests (See Service Manual)
324-326	Subsynthesizer tests (See Service Manual)
327-333	Sum loop tests (See Service Manual)
334-336	RF output tests (See Service Manual)
337-338	Pulse modulator tests (See Service Manual)
339-356	Filter tests (See Service Manual)

Appendix F

Rear Panel AUX Connector

PIN	SIGNAL	FUNCTION
1	Input	Sequence [illegible] location
2	Input	Sequence to memory location
3		Ground
4	Output	[illegible]
5	Output	Switched +5
6		—
7		—
8		—
9		Toggle each time a [illegible]
		re-numbers are sent to [illegible]

Appendix F
Rear Panel AUX Connector Pinout

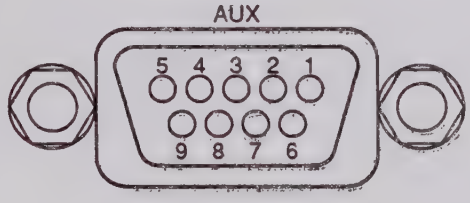

PIN	DIRECTION	FUNCTION
1	Input	Sequence down memory location
2	Input	Sequence up memory location
3		Ground
4	Output	Pen Lift/Blanking
5	Output	Sweep DAC
6		--
7		--
8		--
9	Input	Toggle bright digit between frequency and amplitude fields.

Appendix C

Fluke Sales and Service Centers

Appendix G
Fluke Sales and Service Centers

TECHNICAL SERVICE CENTERS

U.S. Service Locations

California
Fluke Technical Center
16969 Von Karman Avenue
Suite 100
Irvine, CA 92714
Tel: (714) 863-9031

Fluke Technical Center
46610 Landing Parkway
Fremont, CA 94538
Tel: (415) 651-5112

Colorado
Fluke Technical Center
14180 East Evans Avenue
Aurora, CO 80014
Tel: (303) 695-1171

Florida
Fluke Technical Center
550 S. North Lake Blvd.
Altamonte Springs, FL 32701-5227
Tel: (407) 331-2929

Illinois
Fluke Technical Center
1150 W. Euclid Ave.
Palatine, IL 60067
Tel: (708) 705-0500

Maryland
Fluke Technical Center
5640 Fishers Lane
Rockville, MD 20852
Tel: (301) 770-1576

New Jersey
Fluke Technical Center
East 66 Midland Avenue
Paramus, NJ 07652-0930
Tel: (201) 599-9500

Texas
Fluke Technical Center
1801 Royal Lane, Suite 307
Dallas, TX 75229
Tel: (214) 869-2848

Washington
Fluke Technical Center
John Fluke Mfg. Co., Inc.
1420 75th St. S.W.
M/S 6-30
Everett, WA 98203
Tel: (206) 356-5560

International

Argentina
Coasin S.A.
Virrey del Pino 4071 DPTO E-65
1430 CAP FED
Buenos Aires
Tel: 54 1 522-5248

Australia
Philips Customer Support
Scientific and Industrial
23 Lakeside Drive
Tally Ho Technology Park
East Burwood
Victoria 3151

Australia
Philips Customer Support
Scientific & Industrial
25-27 Paul St. North
North Ryde, N.S.W. 2113
Tel: 61 02 888-8222

Austria
Oesterreichische Philips Industrie
Unternehmensbereich Prof. Systeme
Triesterstrasse 66
Postfach 217
A-1101 Wein
Tel: 43 222-60101, x1888

Belgium
Philips & MBLE Associated S.A.
Scientific & Industrial Equip. Div.
Service Department
80 Rue des deux Gares B-1070
Brussels
Tel: 32 2 525 6111

Brazil
Hi-Tek Electronica Ltda.
Al. Amazonas 422, Alphaville
CEP 06400 Barueri
Sao Paulo
Tel: 55 011 421-5477

Canada
Fluke Electronics Canada Inc.
400 Britannia Rd. East, Unit #1
Mississauga, Ontario
L4Z 1X9
Tel: 416-890-7600

Chile
Intronsa Inc.
Casilla 16158
Santiago 9
Tel: 56 2 232-1886, 232-4308

China
Fluke International Corp.
P.O. Box 9085
Beijing
Tel: 86 01 512-3436

Colombia
Sistemas E Instrumentacion, Ltda.
Carrera 13, No. 37-43, Of. 401
Ap. Aereo 29583
Bogota
Tel: 57 232-4532

Denmark
Philips A/S
Technical Service I & E
Strandlodsvej 1A
Postbox 1919
DK-2300
Copenhagen S
Tel: 45 1 572222

Ecuador
Proteco Coasin Cia., Ltda.
P.O. Box 228-A
Ave. 12 de Octubre
2285 y Orellana
Quito
Tel: 593 2 529684

Egypt
Philips Egypt
10, Abdel Rahman el Rafei st.
el. Mohandessin
P.O. Box 242
Dokki Cairo
Tel: 20-2-490922

England
Philips Scientific
Test & Measuring Divis.
Colonial Way
Watford
Hertfordshire WD2 4TT
Tel: 44 923-240511

Finland
OY PHILIPS AB
Central Service
Sinikalliontie 1-3
P.O. Box 11
SF-02631 ESPOO
Tel: 358-0-52572

France
S.A. Philips Industrielle
et Comerciale,
Science et Industry
105 Rue de Paris BP 62
93002 Bobigny, Cedex
Tel: 33-1-4942-8040

Greece
Philips S.A. Hellenique
15, 25th March Street
177 78 Tavros
10210 Athens
Tel: 30 1 4894911

Hong Kong
Schmidt & Co (H.K.) Ltd.
18/FL., Great Eagle Centre
23 Harbour Road
Wanchai
Tel: 852 5 8330222

India
Hinditron Services Pvt. Ltd
1st Floor, 17-B,
Mahal Industrial Estate
Mahakali Road, Andheri East
Bombay 400 093
Tel: 91 22 6300043

Hinditron Services Pvt. Inc.
33/44A Raj Mahal Villas Extn.
8th Main Road
Bangalore 560 080
Tel: 91 812 363139

Hinditron Services Pvt. Ltd.
Field Service Center
Emerald Complex 1-7-264
5th Floor
114 Sarojini Devi Road
Secunderabad 500 003
Tel: 08 42-821117

Hindtron Services Pvt. Ltd.
15 Community Centre
Panchshila Park
New Delhi 110 017
Tel: 011-6433675

Indonesia
P.T. Lamda Trigana
P.O. Box 6/JATJG
Jakarta 13001
Tel: (021) 8195365

Israel
R.D.T. Electronics Engineering, Ltd.
P.O. Box 43137
Tel Aviv 61430
Tel: 972 3 483211

Italy
Philips S.p.A.
Sezione I&E / T&M
Viale Elvezia 2
20052 Monza
Tel: 39-39-363-5342

Japan
John Fluke Mfg. Co., Inc.
Japan Branch
Sumitomo Higashi Shinbashi Bldg.
1-1-11 Hamamatsucho
Minato-ku
Tokyo 105
Tel: 81 3 434-0181

Korea
Myoung Corporation
Yeo Eui Do P.O. Box 14
Seoul 150
Tel: 82 2 784-9942

Malaysia
Mecomb Malaysia Sdn. Bhd.
P.O. Box 24
46700 Petaling Jaya
Selangor
Tel: 60 3 774-3422

Mexico
Mexel Servicios en Computacion
Instrumentacion y Perifericos
Blvd. Adolfo Lopez Mateos No. 163
Col. Mixcoac
Mexico D.F.
Tel: 52-5-563-5411

Netherlands
Philips Nederland
Test & Meetapparaten Div.
Postbus 115
5000 AC Tilburg
Tel: 31-13-352455

New Zealand
Philips Customer Support
Scientific & Industrial
2 Wagener Place
Mt. Albert
Auckland
Tel: 64 9 894-160

Norway
Norsk A/S Philips
I&E Service
Sandstuveien 70
Postboks 1 Manglerud
N 0680 OSLO 6
Tel: 47-2-680200

TECHNICAL SERVICE CENTERS (cont)

Pakistan
International Operations (PAK) Ltd.
505 Muhammadi House
I.I. Chundrigar Road
P.O. Box 5323
Karachi
Tel: 92 21 221127, 239052

Peru
Importaciones & Representaciones
Electronicas S.A.
Avad Franklin D. Roosevelt 105
Lima 1
Tel: 51 14 288650

Philippines
Spark Electronics Corp.
P.O. Box 610, Greenhills
Metro Manila 1502
Tel: 63-2-700-621

Portugal
Philips Portuguese S.A.
I&E Division
Estrada de Outurela-Carnaxide
2795 Linda-A-Velha
Tel: 418 00 71

Singapore
Rank O'Connor's Singapore Pte Ltd
98 Pasir Panjang Road
Singapore 0511
Tel: 65 4737944

South Africa
South African Philips (Pty) Ltd.
Service Department
195 Main Rd
Martindale, Johannesburg 2092
Tel: 27 11 470-5255

Spain
Philips Iberica Sae
Depto. Tecnico Instrumentacion
c/Martinez Villergas 2
28027 Madrid
Tel: 34 1 4042208

Sweden
Philips Kistaindustrier AB
I&E Technical Customer Support
Borgarfjordsgatan 16
S 164 93 Kista
Tel: 46-8-7031000

Switzerland
Philips A.G.
Technischer Kundendienst
Postfach 670
Allmendstrasse 140
CH-8027 Zurich
Tel: 41 1 482211

Taiwan, R.O.C.
Schmidt Electronics Corp.
5th Floor, Cathay Min Sheng
Commercial Building,
344 Min Sheng East Road
Taipei
Tel: 886 2 501-3466

Thailand
Measuretronix Ltd.
2102/31 Ramkamhaeng Rd.
Bangkok 10240
Tel: 66 2 375-2733, 375-2734

Turkey
Turk Philips Ticaret A.S.
Inonu Caddesi 78/80
Posta Kutusu 504-Beyoglu
Istanbul
Tel: 90 1 1435891

Uruguay
Coasin Uruguaya S.A.
Casilla de Correo 1400
Libertad 2525
Montevideo
Tel: 598-2-789015

Venezuela
Coasin C.A.
Calle 9 Con Calle 4, Edif. Edinurbi
Apartado de Correos Nr-70-138
Los Ruices
Caracas 1070-A
Tel: 58 2 241-0309, 241-1248

Federal Republic of Germany
Philips GmbH
Service VSF
Unternehmensbereich Elektronik
fuer Wissenschaft und Industrie
Oskar-Messter-Strasse 18
D-8045 Ismaning
Tel: 49-(0)89-9605-261